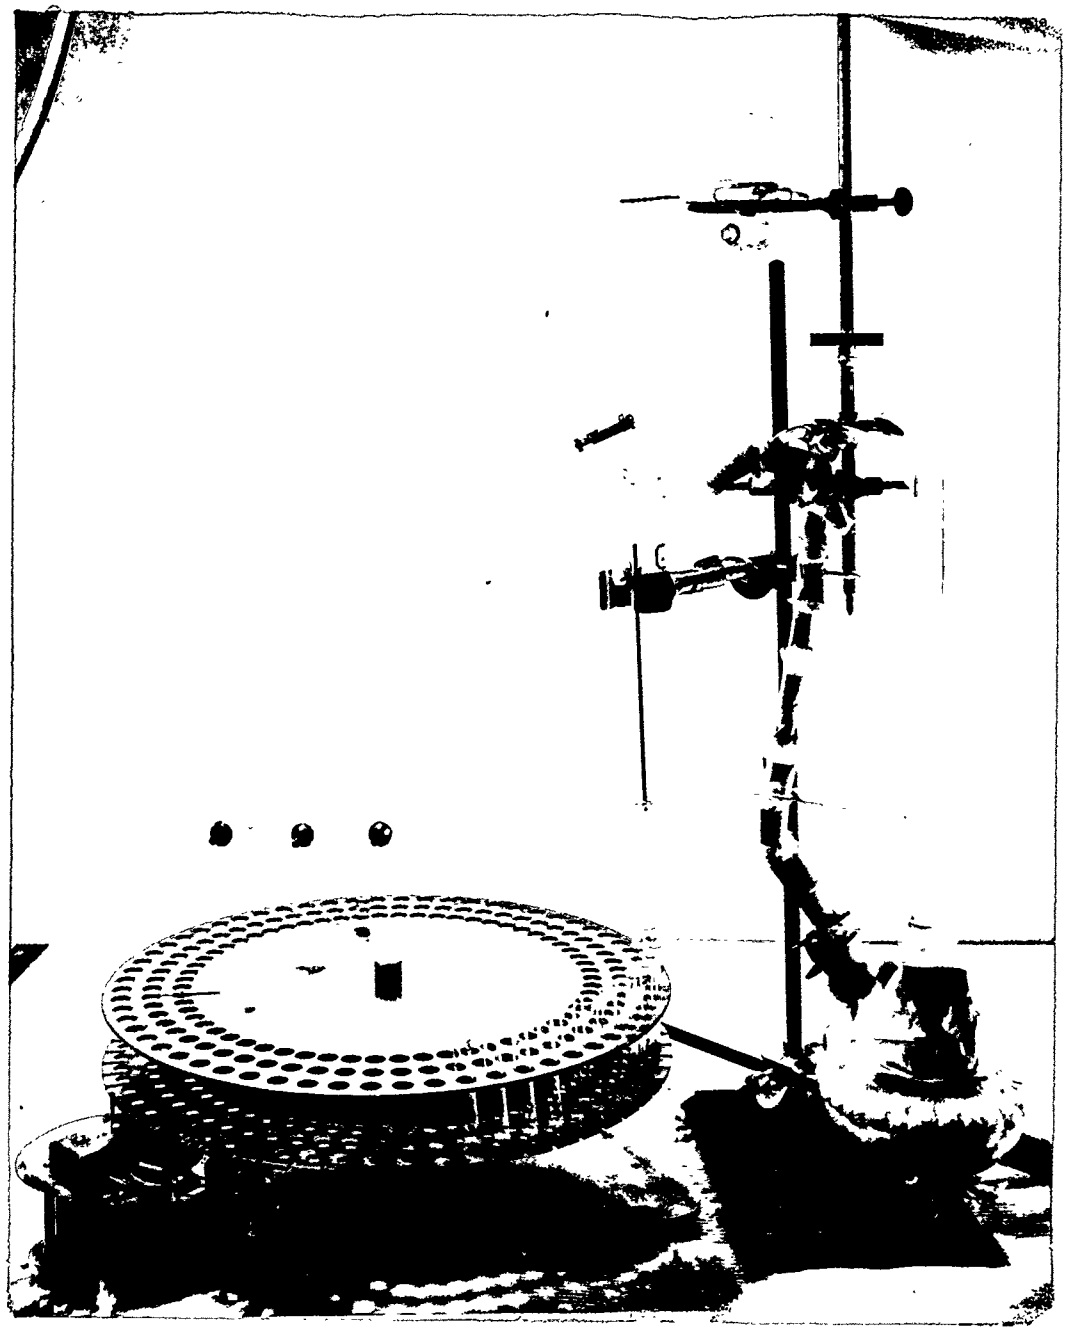

Fig. 19

Ion exchange column with elution apparatus and automatic sample collection mechanism for separation of actinide and lanthanide elements.