


CT Scan of Duracell® Battery



31 μm effective voxel size, 4x magnification

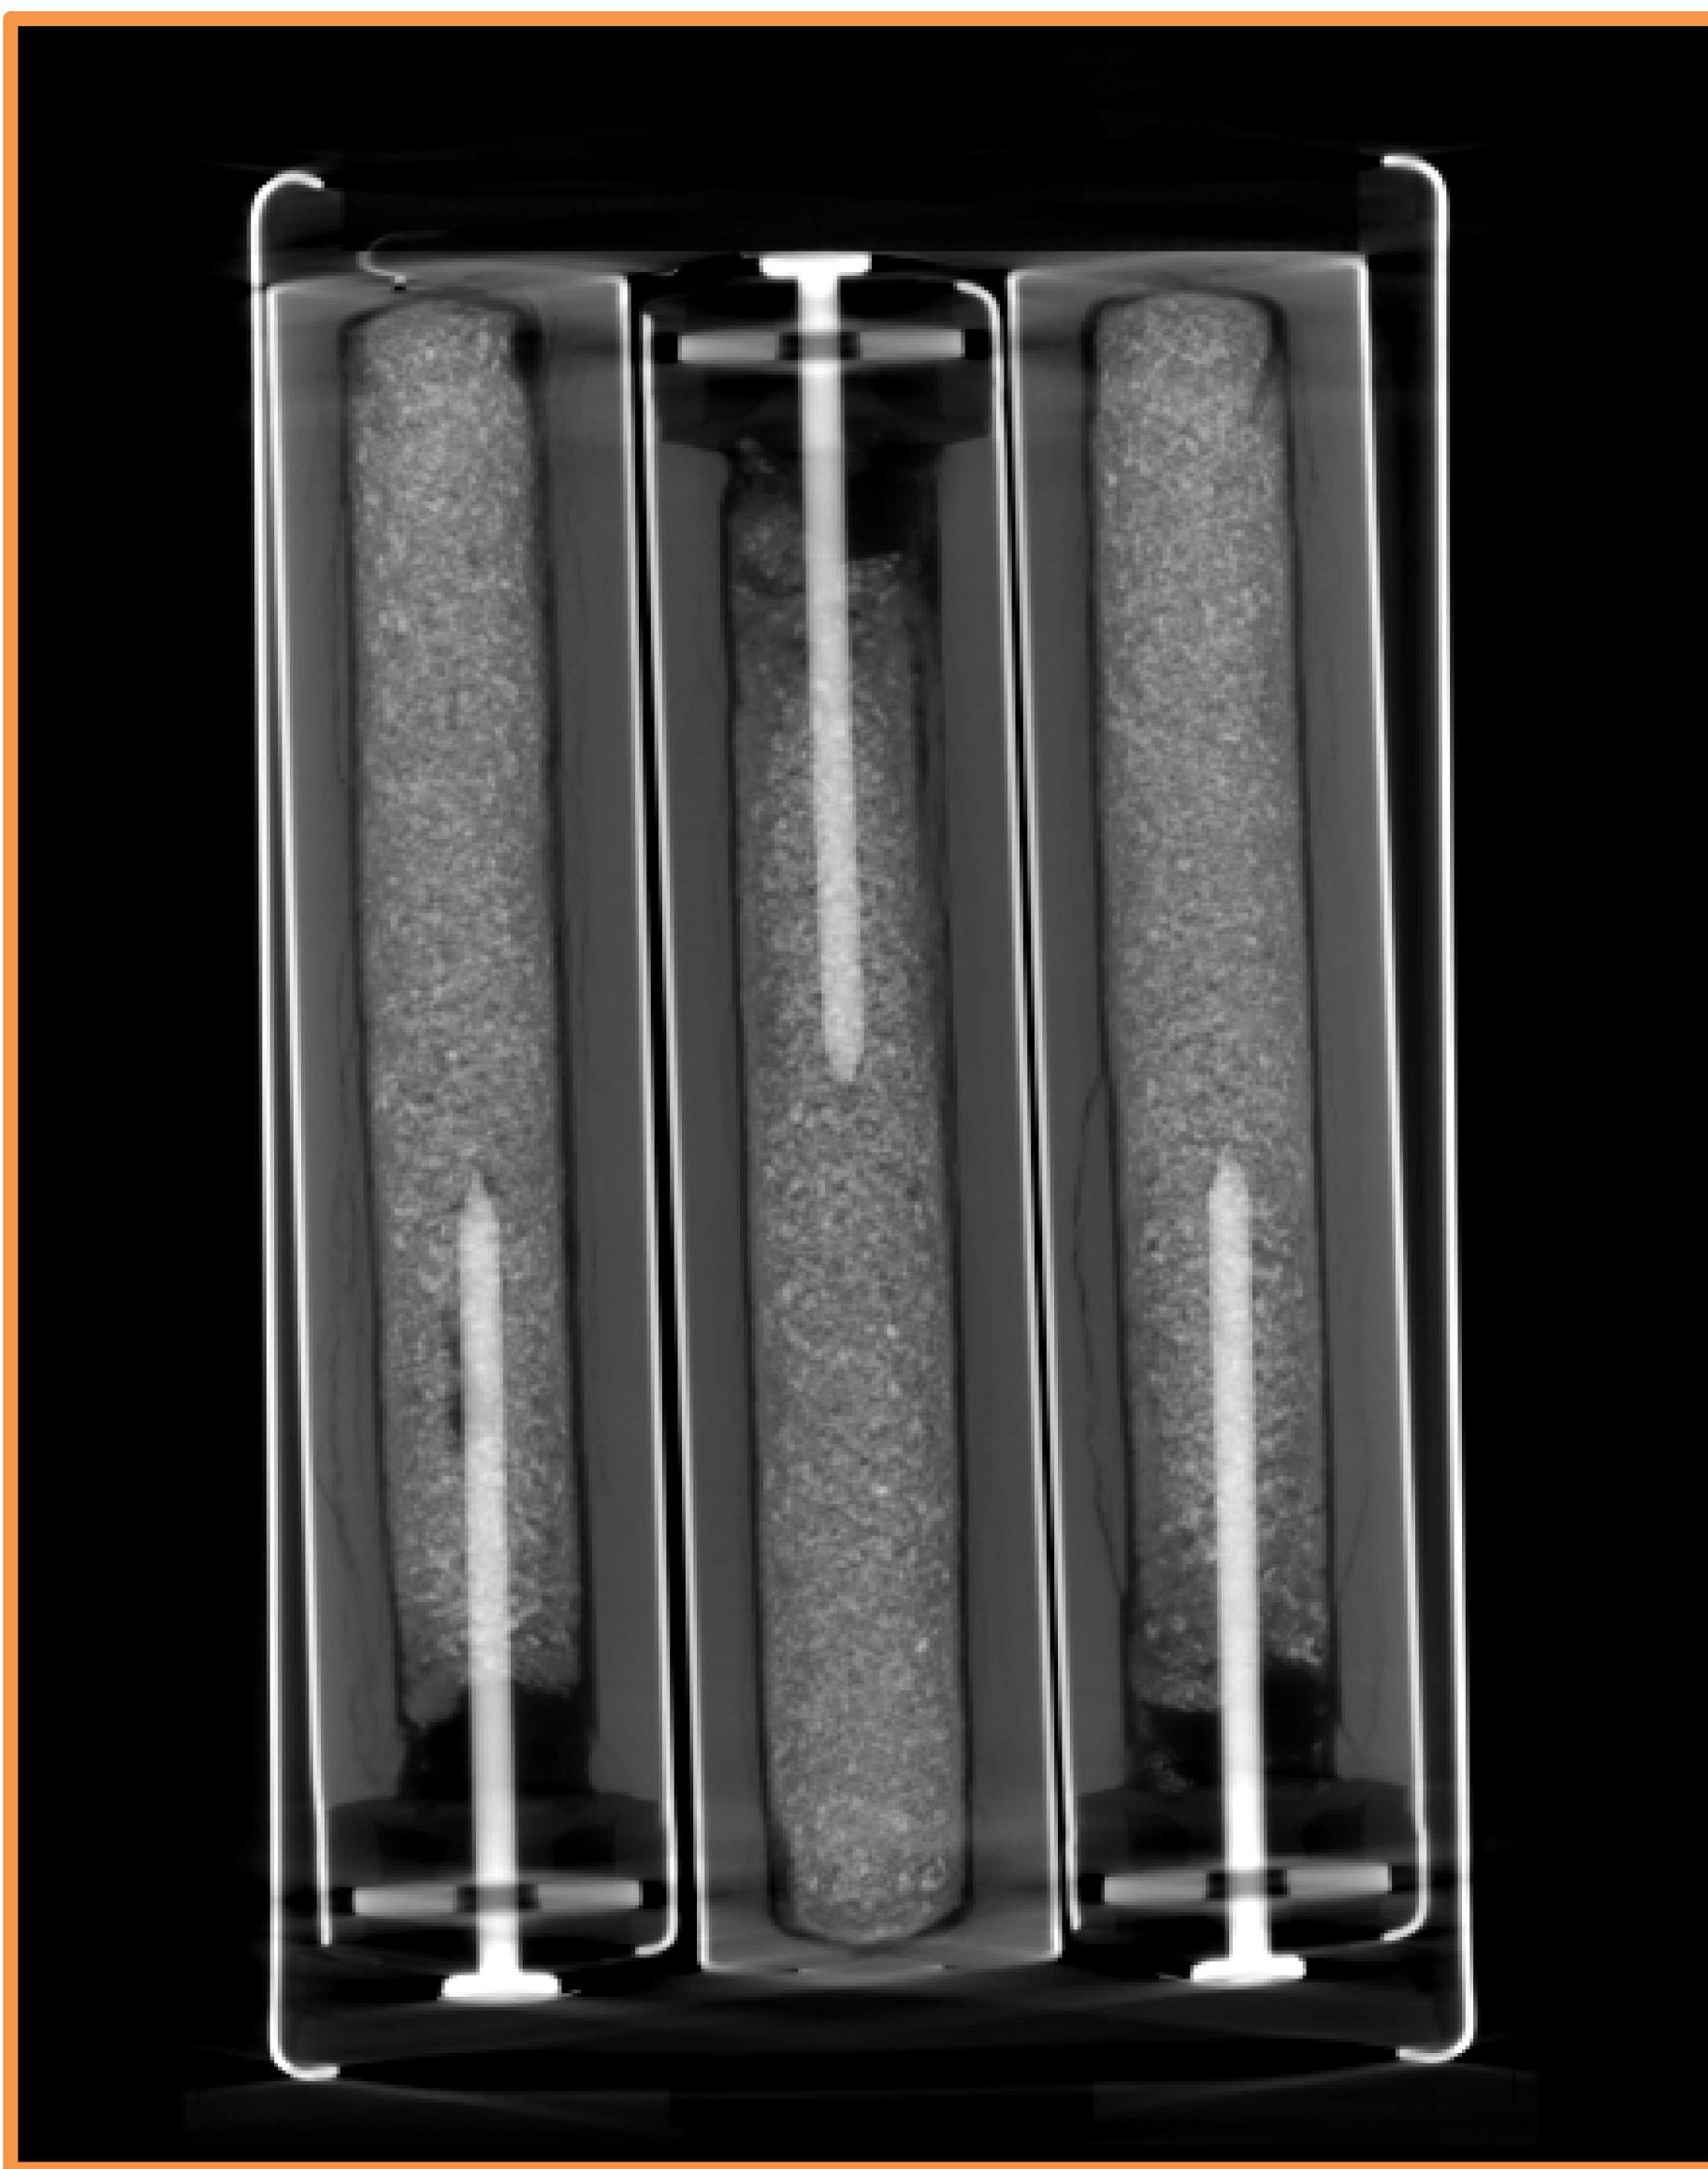

The battery was shot using a 225 kV X-Ray Worx system with a Varian 2520DX detector

CT Scan of an Amethyst Geode


42 μm effective voxel size, 3x magnification

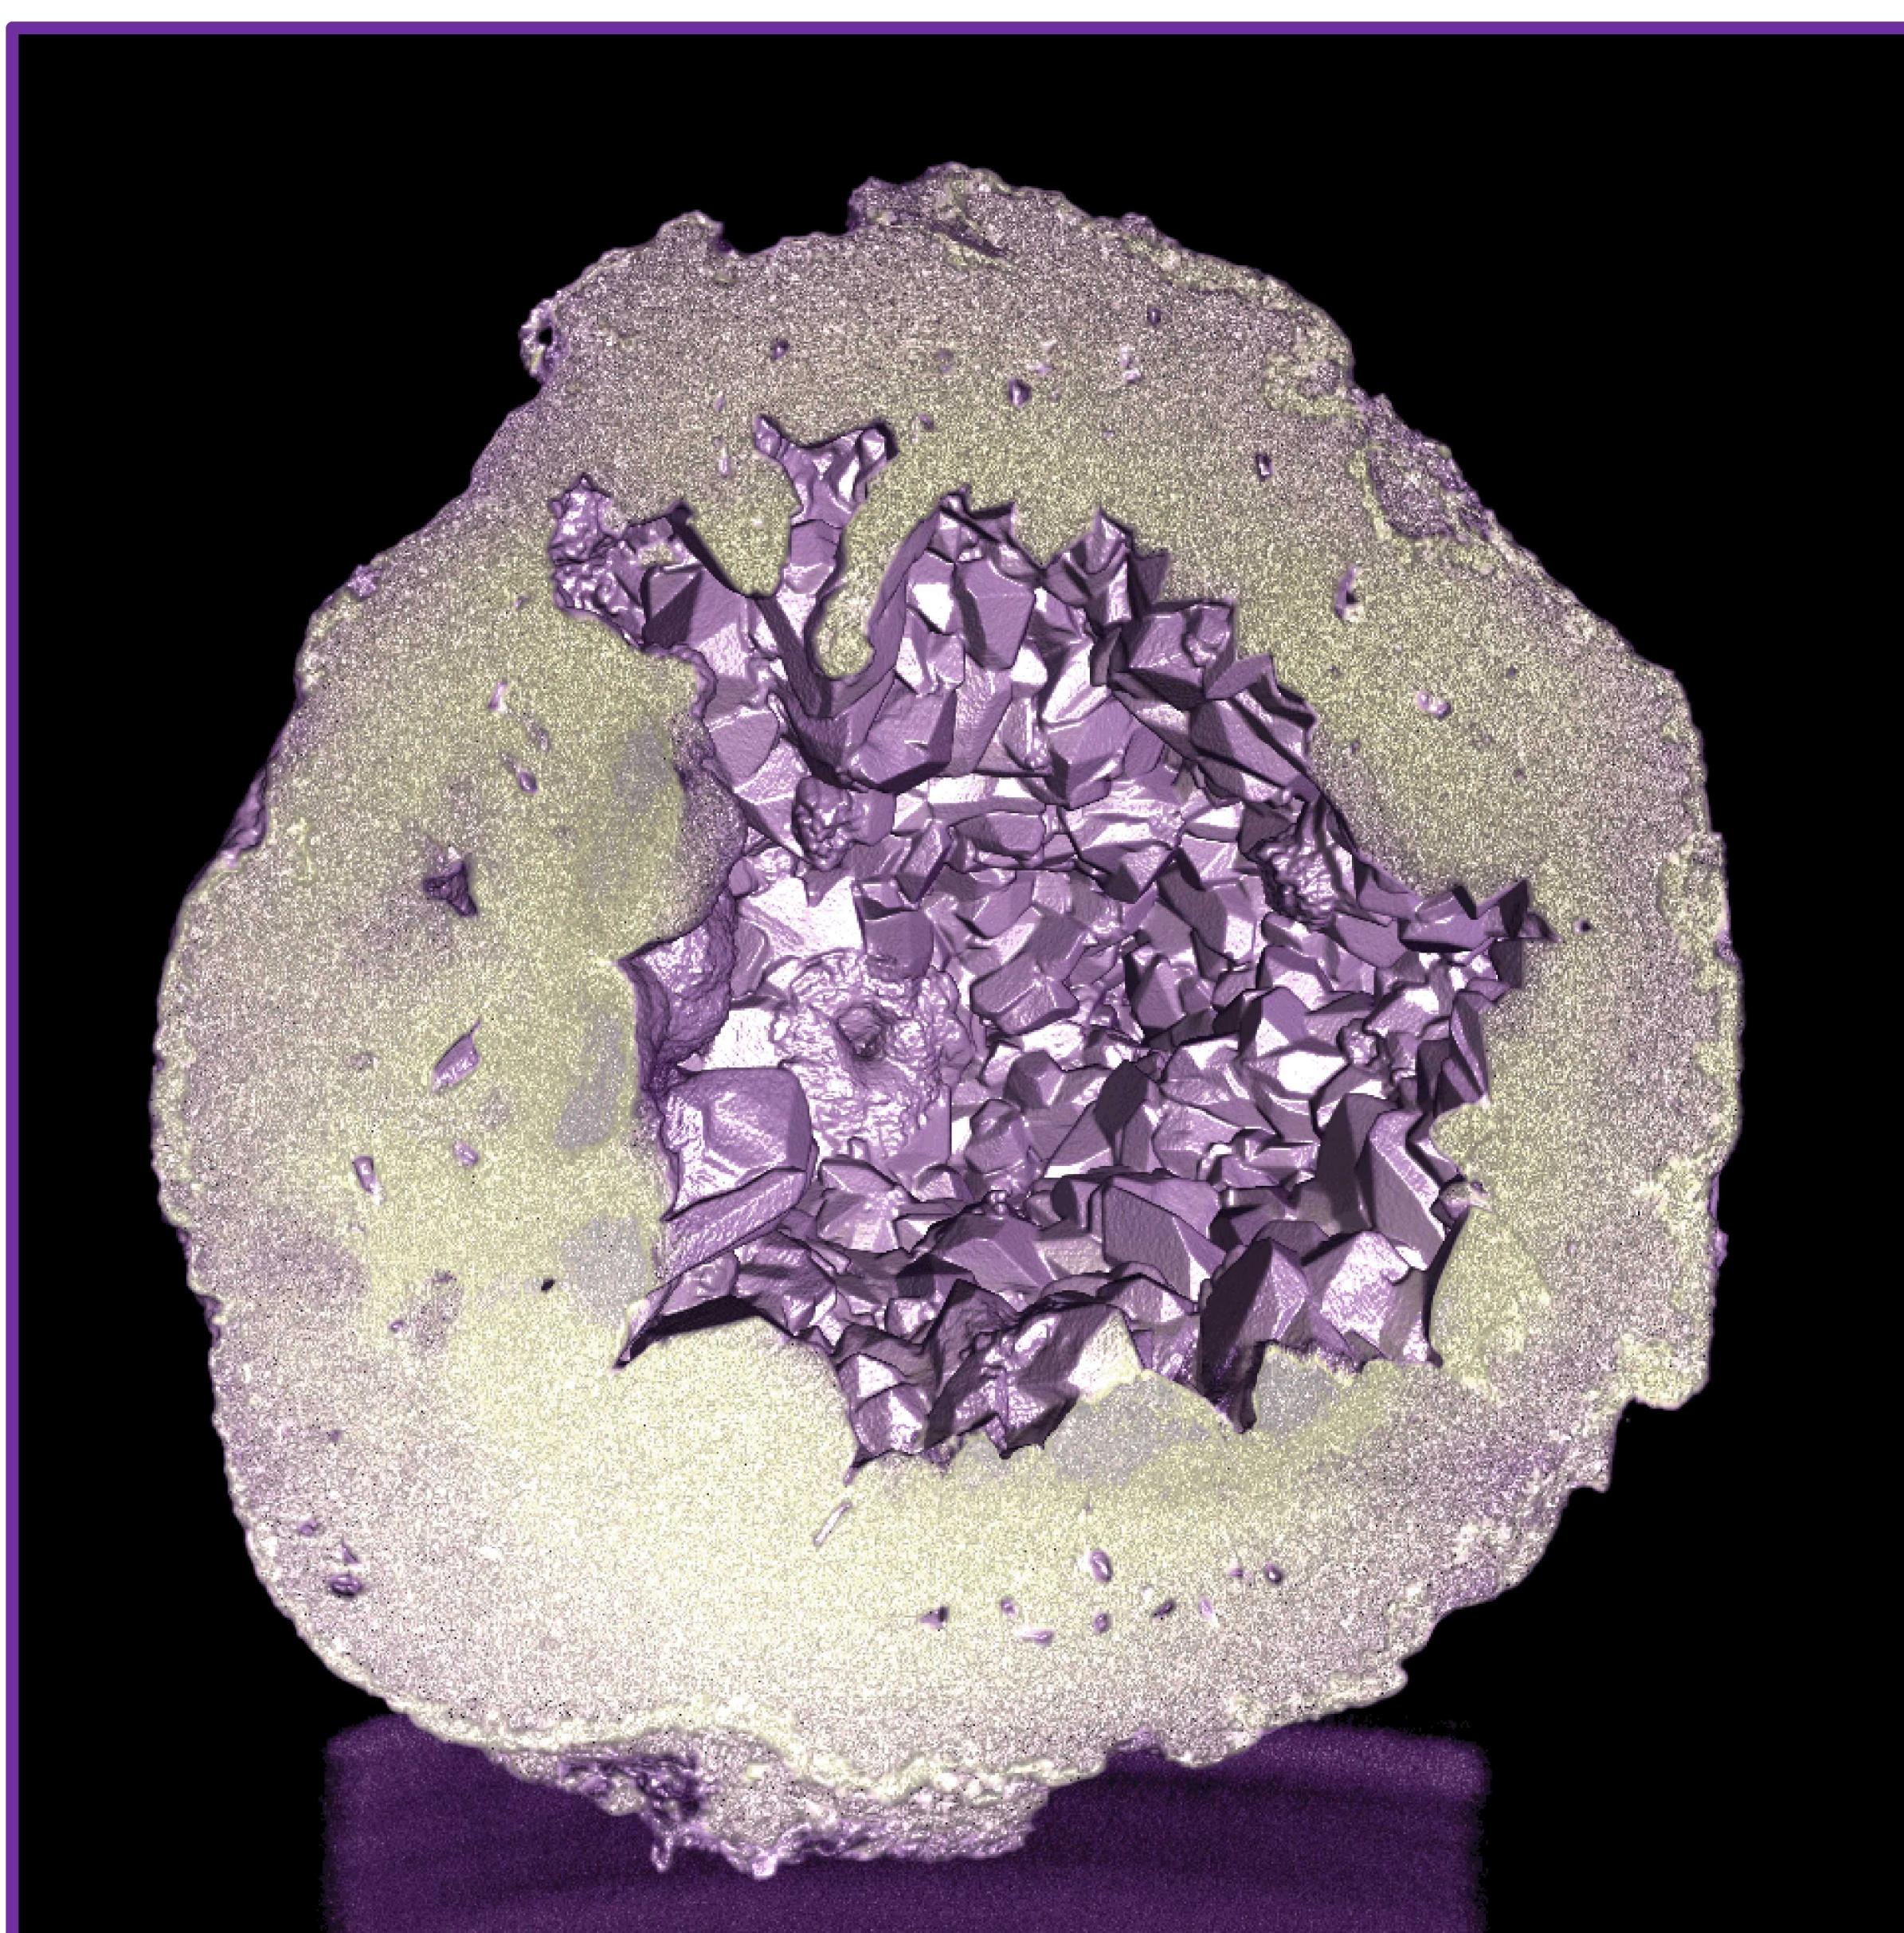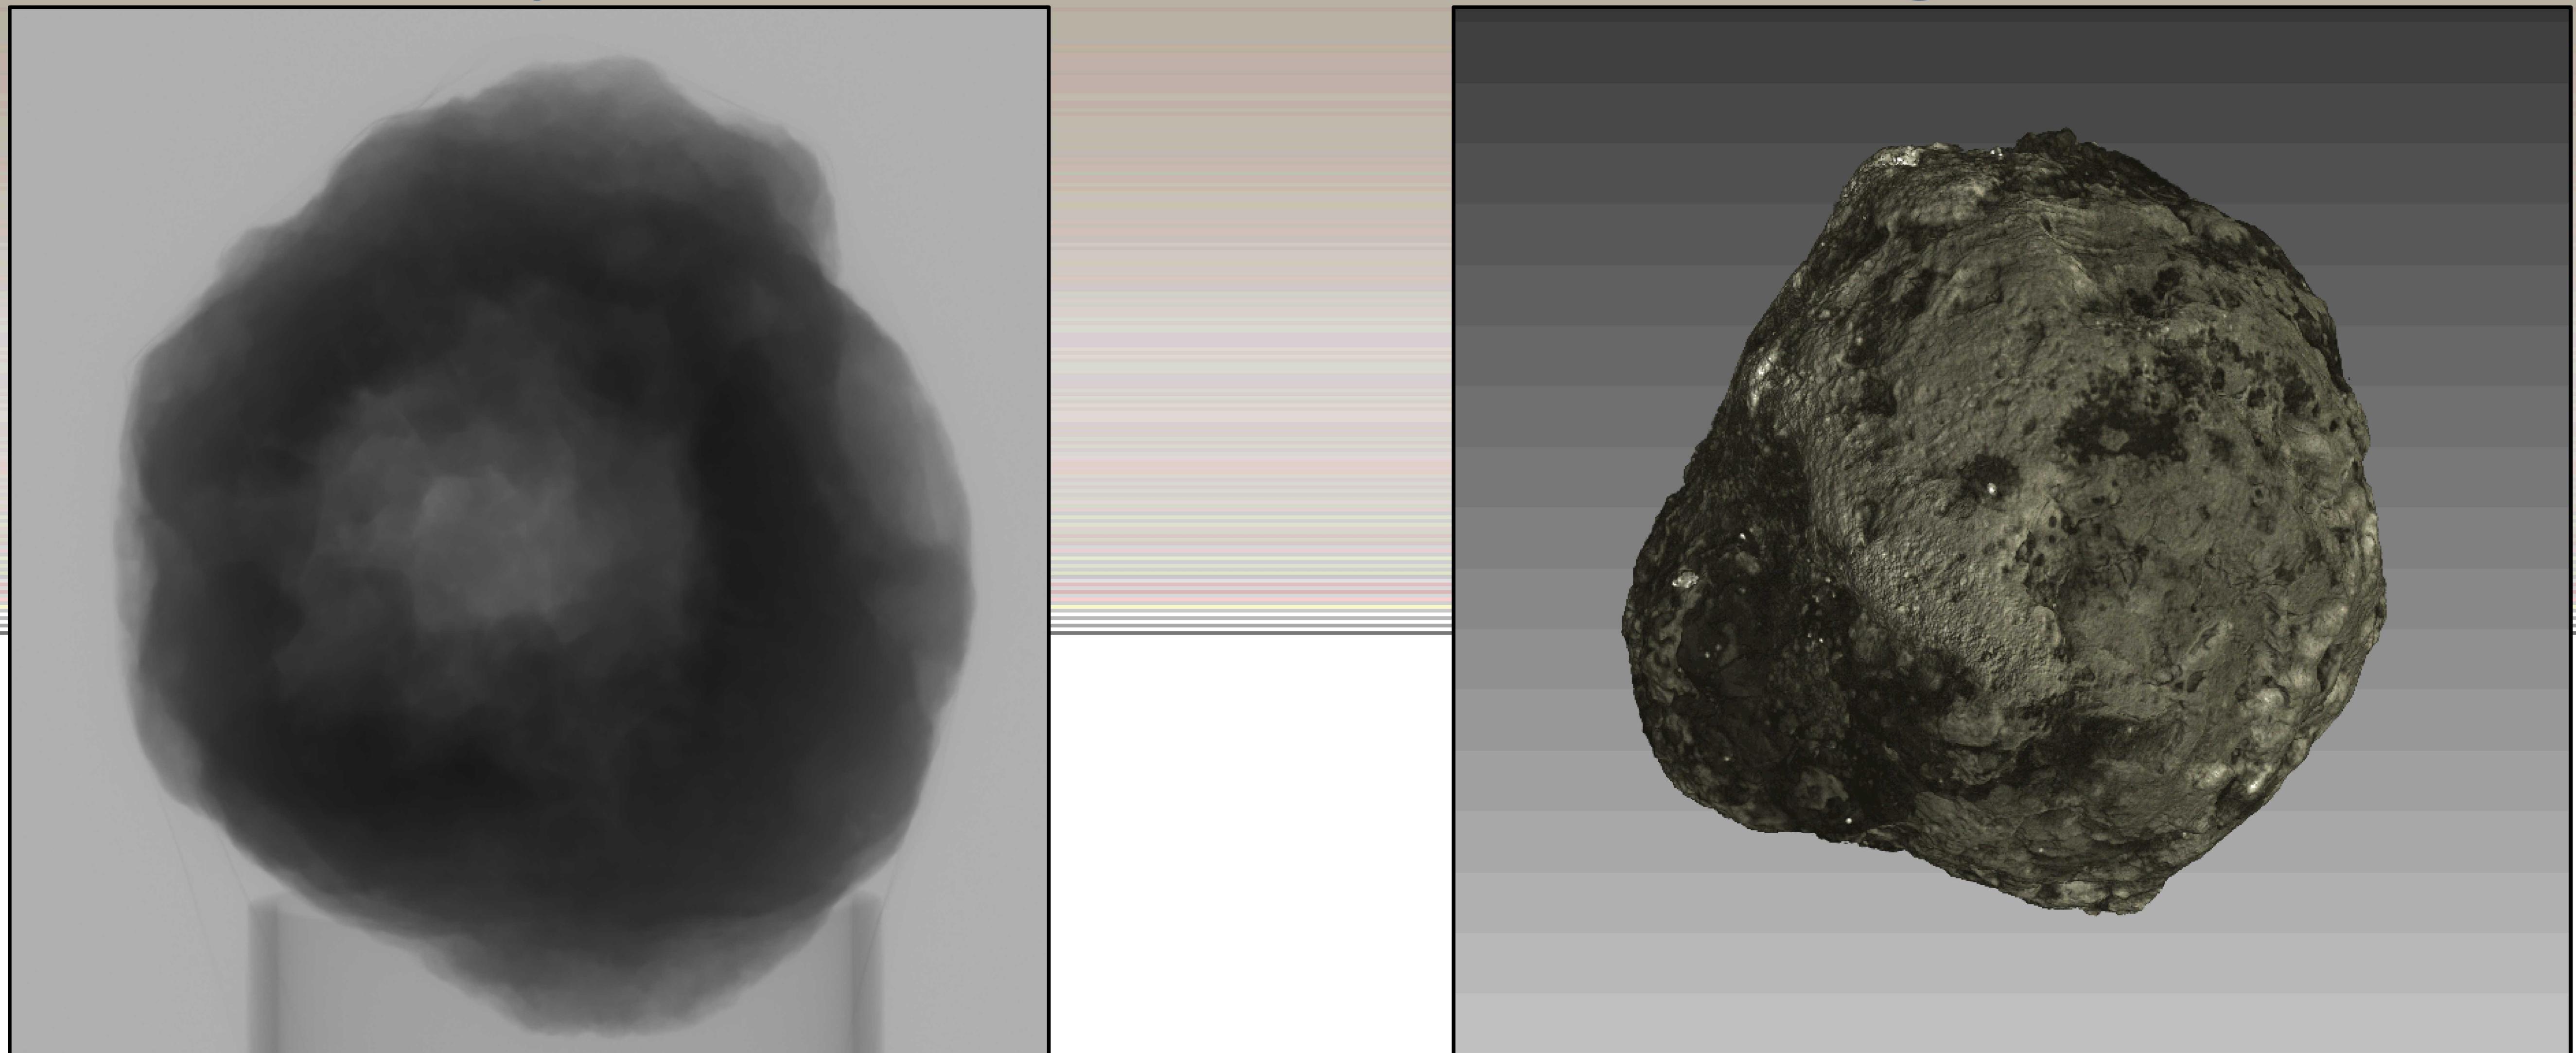

The Geode was shot using a 225 kV X-Ray Worx system with a Varian 2520DX detector

CT Scan of an Additive Manufactured Pull Samples


5.7 μm effective voxel size, 14x magnification

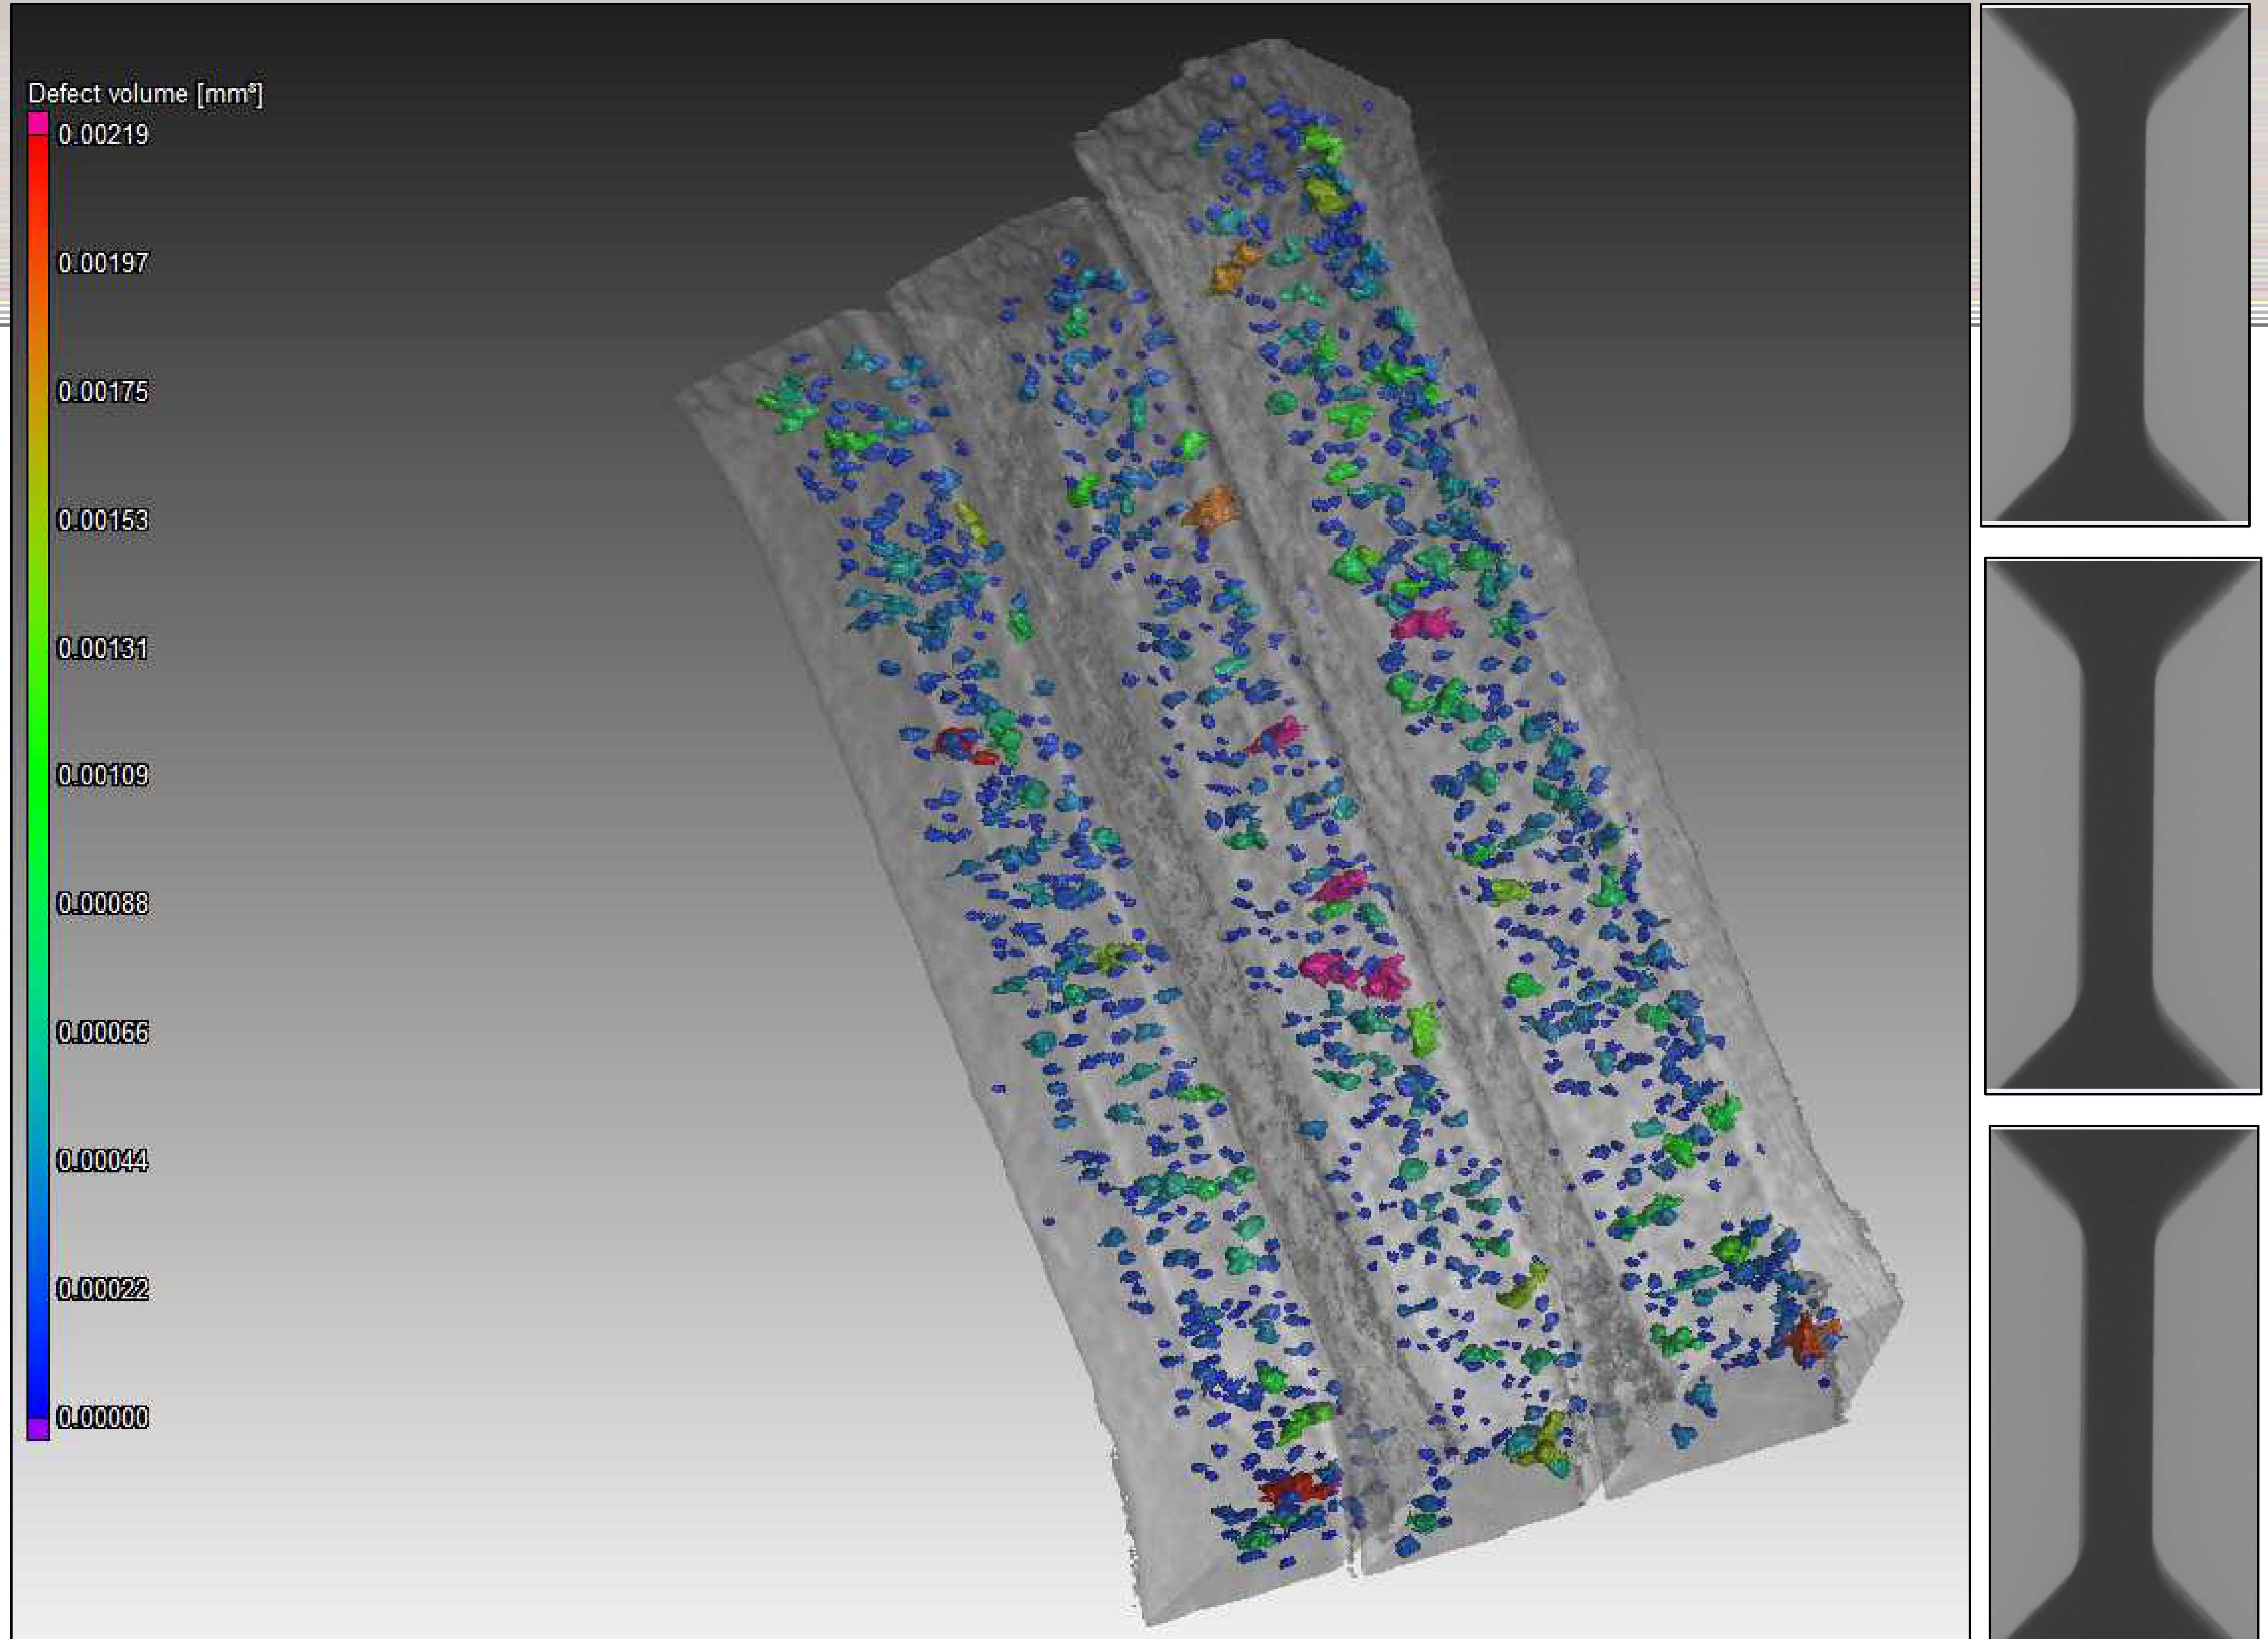

Porosity Analysis Application
The samples were shot using a 225 kV X-Ray
Worx system with a Varian 2520DX detector

CT Scan of an Additive Manufactured Polyhedron

30 μm effective voxel size, 4x magnification

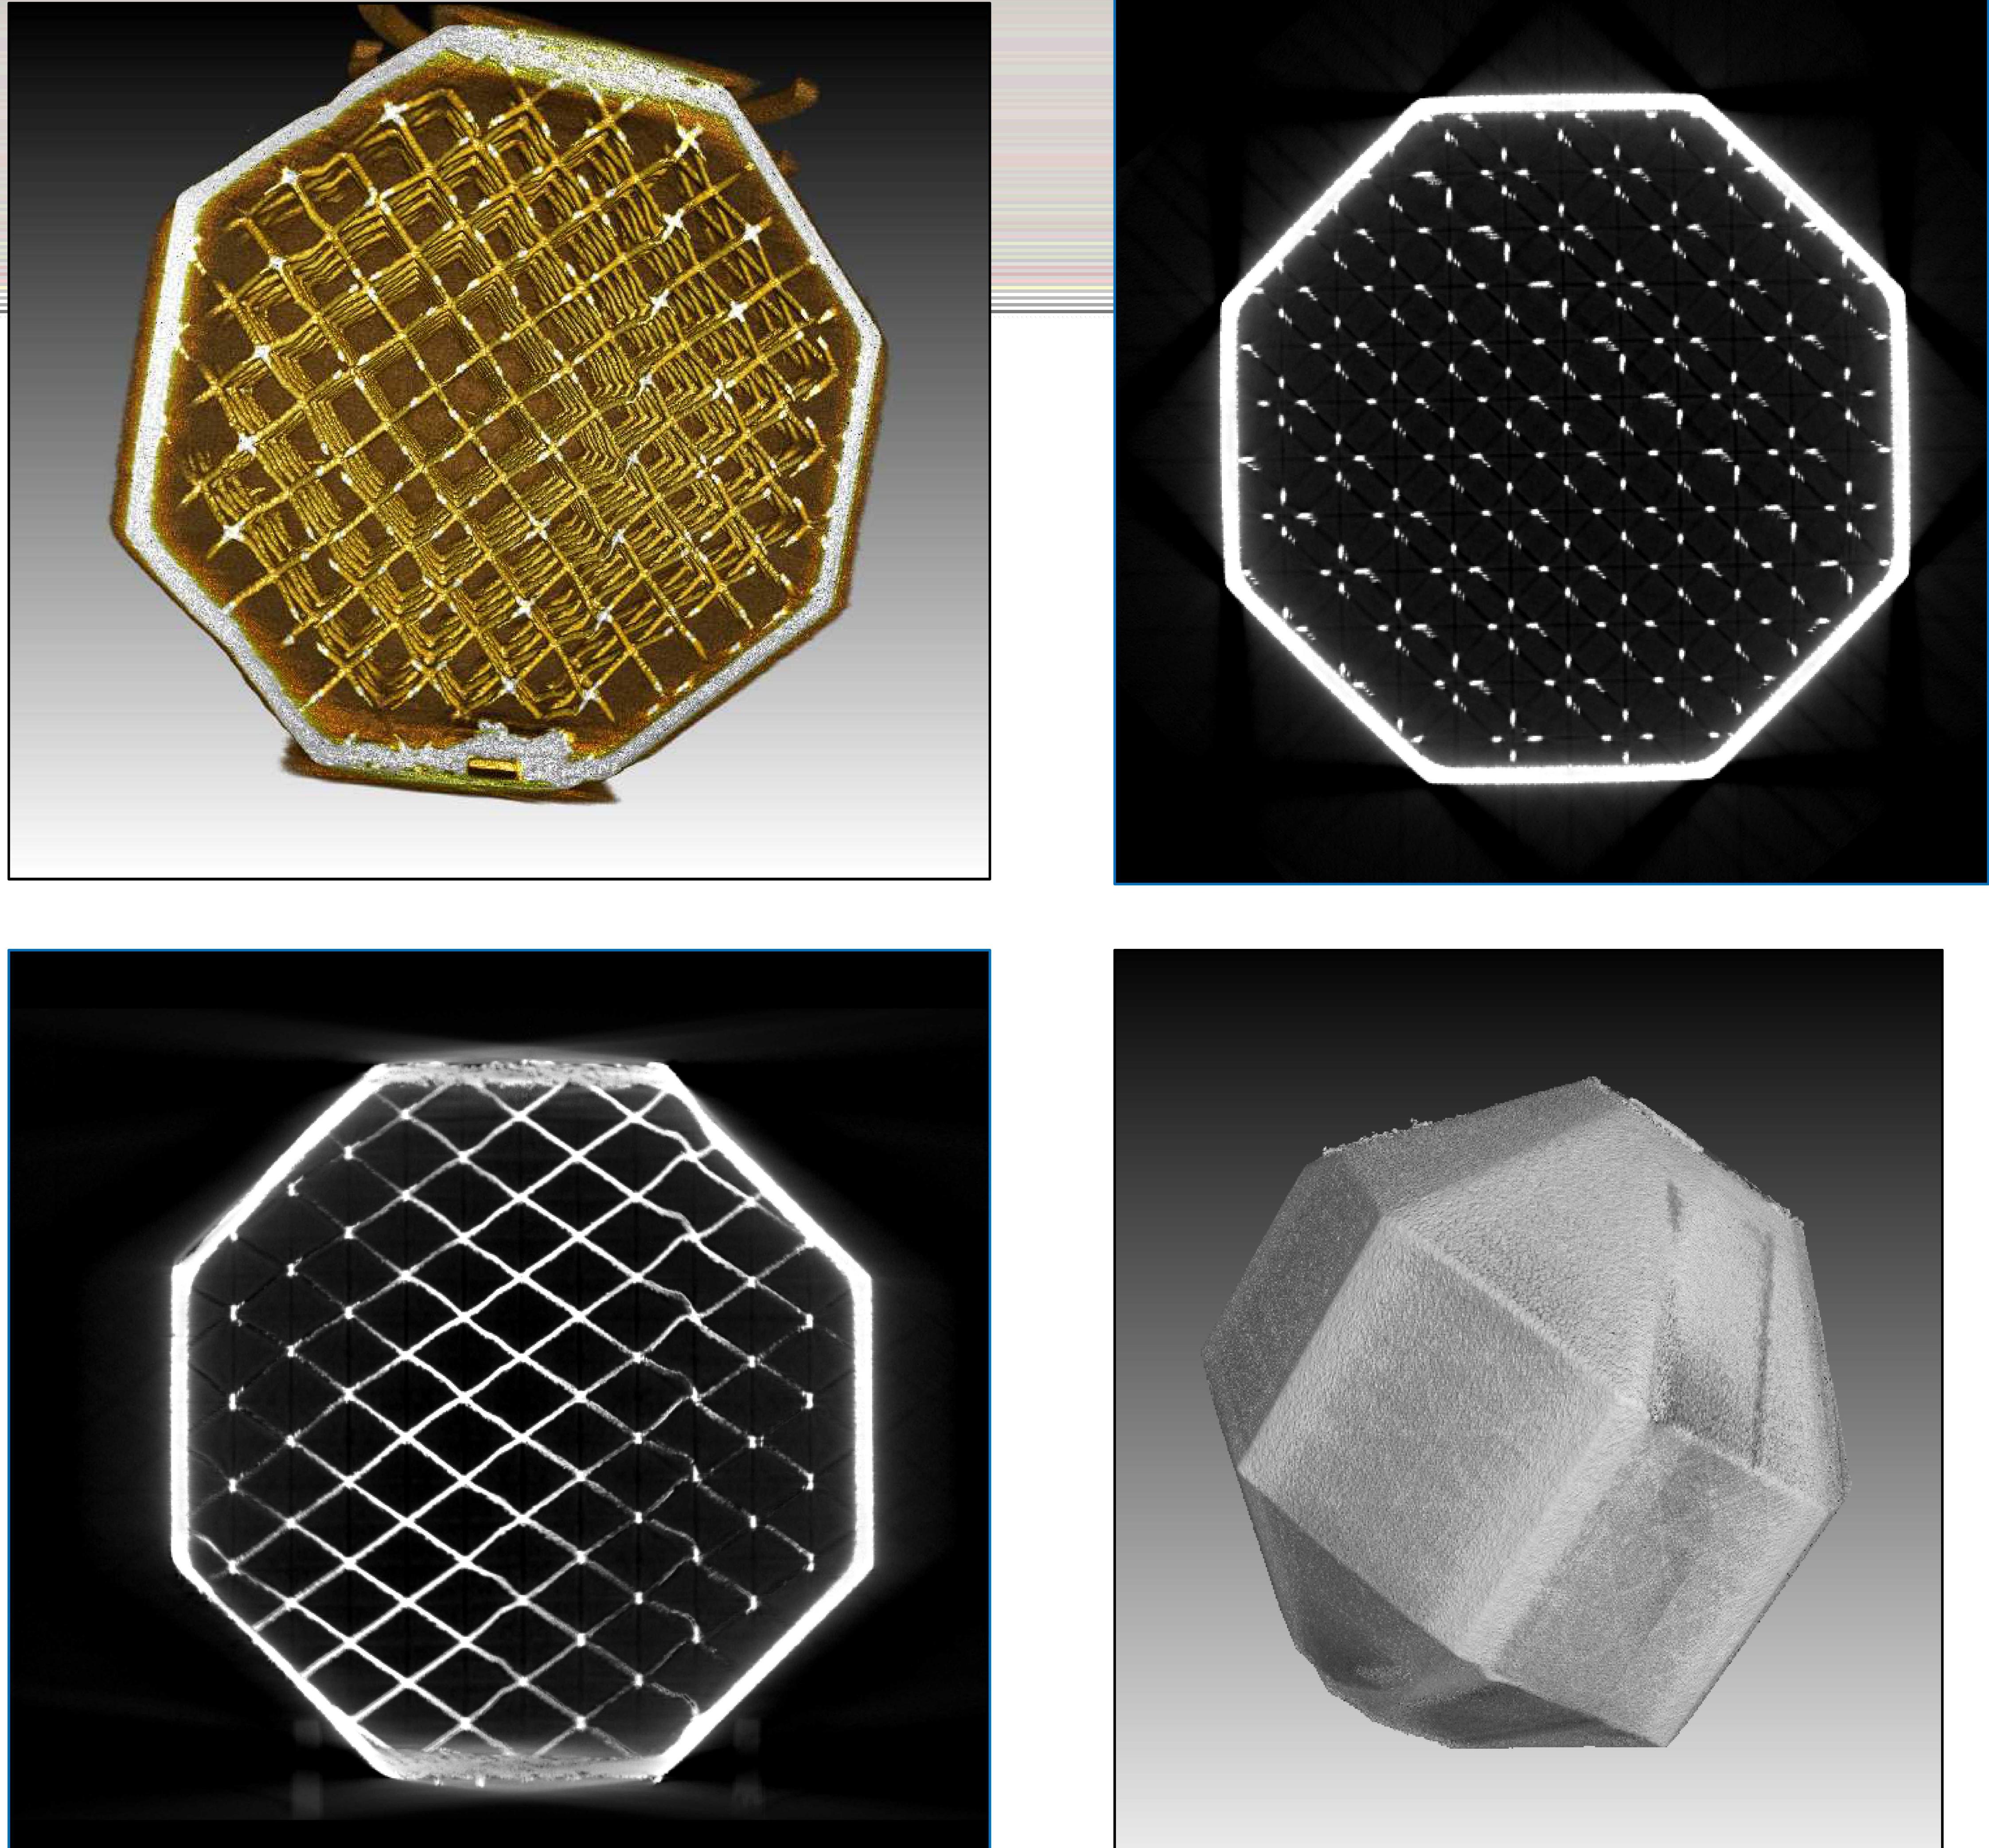

The sample was shot using a 225 kV X-Ray Worx system with a Varian 2520DX detector