

By acceptance of this article, the publisher or recipient acknowledges the U.S. Government's right to retain a nonexclusive, royalty-free license in and to any copyright covering the article.

Conf-830559--1

**MASTER**

ORNL TRU-WASTE-ASSAY SYSTEM\*

CONF-830559--1

DE83 012592

F. J. Schultz and K. W. Haff

Oak Ridge National Laboratory  
Oak Ridge, Tennessee 37830

and

J. T. Caldwell, D. A. Close, T. H. Kuckertz,  
W. E. Kunz, and J. C. Pratt

Los Alamos National Laboratory  
Los Alamos, New Mexico 87544

---

\*Research sponsored by the Office of Defense Waste Management, U.S. Department of Energy, under contract W-7405-eng-26 with the Union Carbide Corporation.

#### DISCLAIMER

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.

DISTRIBUTION OF THIS REPORT IS UNLIMITED

## ORNL TRU WASTE ASSAY SYSTEM\*

F. J. Schultz and K. W. Haff

Oak Ridge National Laboratory, P.O. Box X  
Oak Ridge, Tennessee 37830

J. T. Caldwell, D. A. Close, T. H. Kuckertz,  
W. E. Kunz, and J. C. Pratt

Los Alamos National Laboratory  
Los Alamos, New Mexico 87544

### INTRODUCTION

ORNL transuranic (TRU) waste is retrievably stored in 208-L (55-gal) stainless steel drums below grade in weather-resistant structures under controlled surveillance. Due to the limited space available for storage, it is advantageous and cost effective to reduce the volume of TRU waste retrievably stored. Waste containing less than 100 nCi/g transuranics (alpha-emitting radionuclides of atomic number greater than 92 and half-lives greater than 20 y)<sup>1</sup> may be disposed of as low-level waste, while waste containing greater than 100 nCi/g transuranics must be retrievably stored.

Classification of the ORNL waste into "TRU" and "non-TRU" is required for proper disposition. The task of classifying the waste is further complicated by the score of TRU isotopes contained in the waste. Four independent TRU-waste-generating streams have contributed to the large array of TRU isotopes. The isotopes present, both TRU and non-TRU, in significant quantities include  $^{233}\text{U}$ ,  $^{235}\text{U}$ ,  $^{238}\text{U}$ ,  $^{237}\text{Np}$ ,  $^{238}\text{Pu}$ ,  $^{239}\text{Pu}$ ,  $^{240}\text{Pu}$ ,  $^{241}\text{Pu}$ ,  $^{242}\text{Pu}$ ,  $^{241}\text{Am}$ ,  $^{242}\text{Cm}$ ,  $^{246}\text{Cm}$ , and  $^{252}\text{Cf}$ . Some 45 additional radionuclides in lesser quantities have been identified.

---

\*By acceptance of this article, the publisher or recipient acknowledges the U.S. Government's right to retain a nonexclusive, royalty-free license in and to any copyright covering the article.

ORNL has been selected as the demonstration site for a new trans-uranic neutron assay system developed at the Los Alamos National Laboratory. The major objectives of the cooperative interlaboratory program is to field test, calibrate, and evaluate the neutron interrogation system, to provide a demonstration and training facility for DOE of this sophisticated technology, to reduce the volume of TRU waste stored at ORNL, and to provide positive identification of the radionuclide content of the ORNL TRU waste.

In order to meet these objectives, a two-tier assay system utilizing the LANL neutron interrogation assay system and an upgraded gamma-ray drum scanner has been employed. This paper will describe each assay technique and the results obtained from the examination of authentic ORNL TRU waste.

#### NEUTRON INTERROGATION ASSAY SYSTEM (NIAS)

The NIAS is both a pulsed, active-neutron interrogation (differential dieaway technique) system and a passive neutron measurement system with the capability of detecting passive neutron totals and passive coincident neutrons and measuring passive neutron multiplicities. A detailed description of the system may be found in the references.<sup>2,3</sup>

The pulsed active portion of the assay determines the fissile component of the drum's TRU isotope content. The coincident passive neutron measurement determines the spontaneous fission component and the passive total neutron measurement, after accounting for the spontaneous fission contribution, can be used to estimate all other TRU isotope contributions. The neutron multiplicity measurements serve to identify which spontaneous fission isotopes are present in significant quantities.

The NIAS passive neutron measurements provide an upper-limit estimate of total TRU activity contained in each drum. Estimates of total spontaneous fission activity and total fissile mass are also obtained. This information is usually sufficient for categorization of a waste drum.

#### GAMMA DRUM SCANNER

The gamma drum scanner used in the assay system is an upgraded Canberra Segmented Drum Scanner Model 2220B. The effects of vertical and radial inhomogeneities are reduced, respectively, by scanning individual horizontal segments along the vertical axis of the drum and by rotating the drum on a turntable at a constant speed. Each active assay scan is corrected for the drum's varying mass absorption coefficient by measuring a gamma source through an empty drum and the waste matrix.

The present assay scheme provides for all drums to be qualitatively scanned for gamma-emitting radioisotope identification. However, only those drums which cannot be positively identified by the NIAS as possessing less than 100 nCi/g TRU concentration will be quantitatively scanned.

#### RESULTS

The ORNL drums surveyed by the NIAS in FY82 are presented in Table 1. In this summary, the total fissile mass is expressed in milligram equivalents of  $^{235}\text{U}$ , while the passive neutron data is summarized in terms of a total neutron source in units of neutrons/second (n/s).

Table 1. ORNL TRU waste drum data summary<sup>4</sup>

Neutrons/s	Fissile mass, Uranium-235 equivalent (mg)					
	0-15	15-50	50-100	100-300	300-1000	>1000
<10 <sup>1</sup>	8	-	1	-	1	-
10 <sup>1</sup> -10 <sup>2</sup>	-	-	-	3	-	1
10 <sup>2</sup> -10 <sup>3</sup>	1	-	1	1	7	7
10 <sup>3</sup> -10 <sup>4</sup>	2	3	2	-	5	7
10 <sup>4</sup> -10 <sup>5</sup>	6	8	4	6	2	7
10 <sup>5</sup> -10 <sup>6</sup>	6	9	1	2	1	1
>10 <sup>6</sup>	4	1	5	1	-	-
TOTAL	27	21	14	13	16	23

From the 114 drums assayed to date, a total of nine drums contain less than 10 nCi/g TRU isotopes based on the combined passive and pulsed active neutron measurements. These TRU waste drums are listed in Table 2.

Table 2. ORNL waste drums containing &lt;10 nCi/g TRU activity

Drum ATN	Total mass (mg <sup>235</sup> U eq.)	Total neutron source (n/s)
1945	3 ± 1	<4
1921	2 ± 1	<4
1924	2 ± 1	<4
1922	5 ± 2	<2
1919	6 ± 2	<2
1208	2 ± 2	<2
1788 <sup>a</sup>	74 ± 5	<3
2101	17 ± 2	<5
1923	2 ± 1	<5

<sup>a</sup>The passive data was used to establish the principal TRU isotope to be <sup>233</sup>U in this drum.

## MATRIX COMPENSATION

Matrix compensation involves the effect of the non-TRU contents of the drums (combustibles, glassware, iron, etc.) on both passive and active neutron measurements.

A general technique for matrix compensation has been established. It is based on the pulsed active thermal neutron flux monitor data. Two parameters can be extracted from the data that, respectively, are single functions of the matrix moderating mass and the matrix absorber mass. These two parameters, the extrapolated zero-time thermal neutron flux intensity ( $A_0$ ) and the thermal neutron lifetime ( $T_{1/2}$ ), are obtained from an exponential least squares fit to the thermal neutron flux monitor data.

The data shown in Fig. 1 is presented in terms of the differential-time zero flux intensity ( $\Delta A_0$ ) relative to an empty drum versus the differential thermal neutron lifetime ( $\Delta T_{1/2}$ ) relative to an empty drum. The presence of absorbing materials in a drum produces a decrease in  $T_{1/2}$  and, consequently,  $\Delta T_{1/2} = T_{1/2}$  (empty drum) -  $T_{1/2}$  (waste drum).

The 113 ORNL TRU waste drums are depicted by the black circles. The 14 matrix standards are outlined by ovals. The numbers are the measured matrix correction values required to obtain the proper assay of a standard fissile sample within the indicated standard matrix. It appears that only a relatively small portion of the ORNL waste drums will require significant matrix corrections.

## REPRODUCIBILITY OF THE ACTIVE NEUTRON MEASUREMENTS

Table 3 illustrates the internal consistency of the pulsed active neutron measurements made on a single drum spanning a three-month period. This intrinsic repeatability demonstrates the basic high quality of the neutron data.

# Fig. 1. ORNL DRUM ASSAY

MATRIX CORRECTION FACTORS

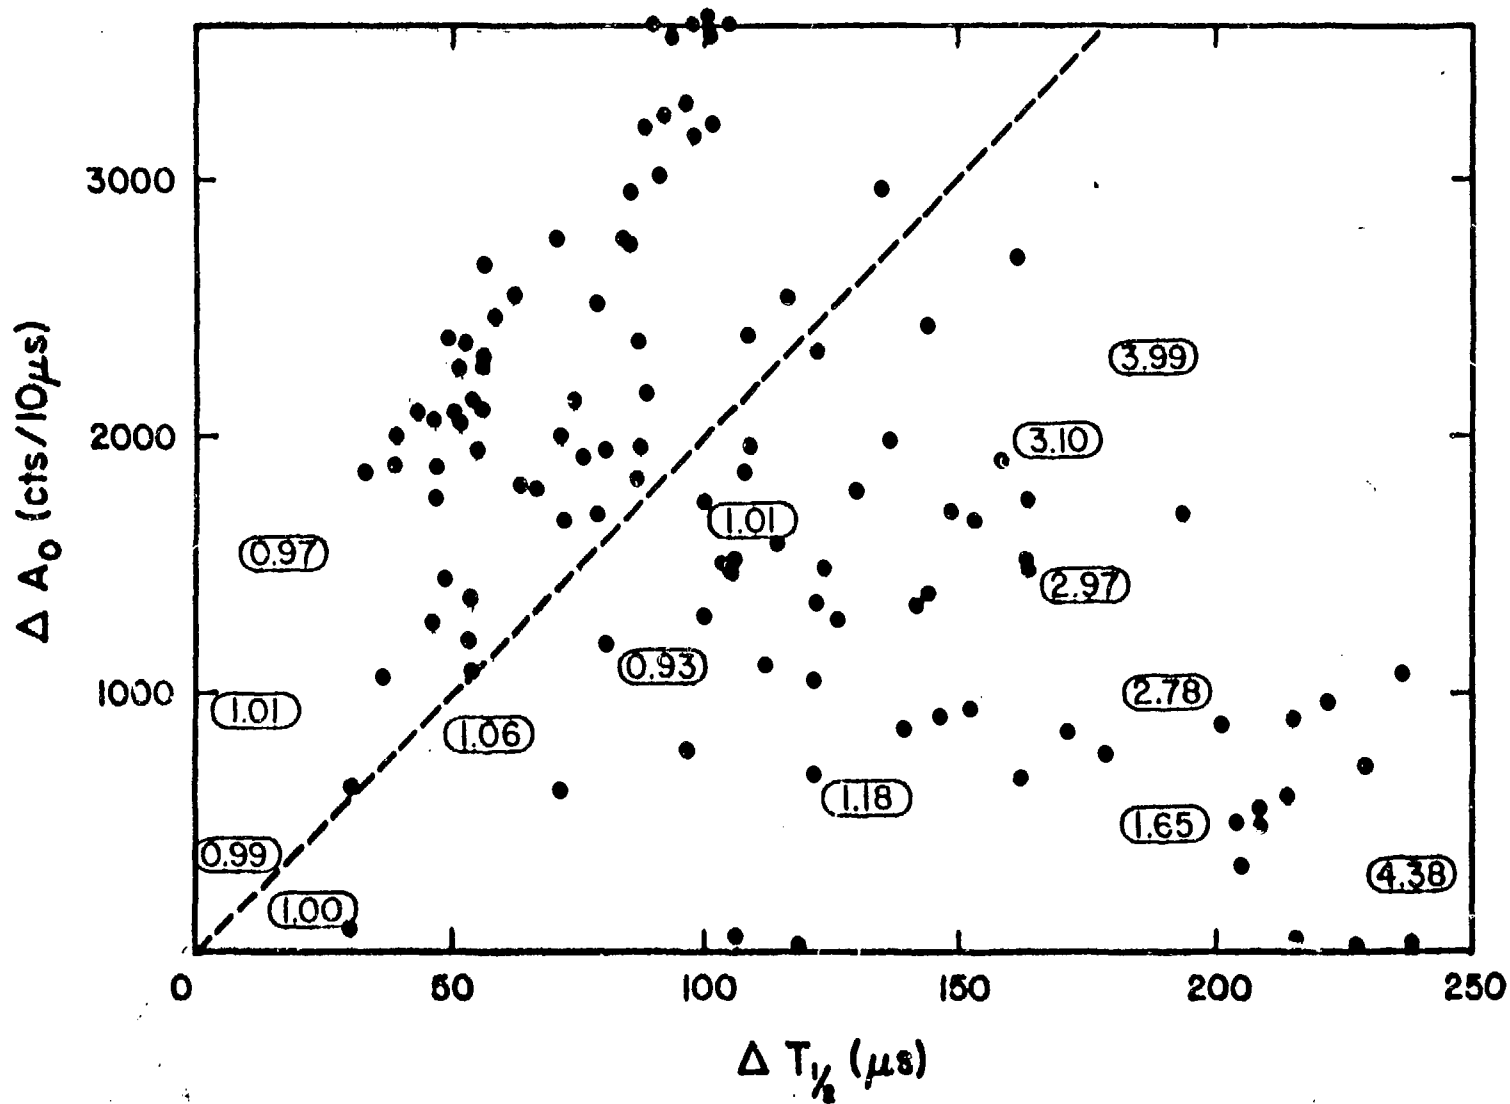


Table 3. Active neutron data for drum 1772

Date	SHTOT/FM	A <sub>o</sub>	T <sub>1/2</sub>
7/16/82	3.37	4500	509
7/22/82	3.33	4264	521
7/22/82	3.30	4232	524
7/22/82	3.30	4332	521
7/22/82	3.33	4255	521
7/22/82	3.34	4367	519
9/22/82	3.28	4530	518
9/22/82	3.28	4613	514
Average	3.32 ± 0.03	4387 ± 134	518 ± 4

## NEUTRON MULTIPLICITY MEASUREMENTS

Table 4 presents samples of neutron multiplicity data obtained using SYSTOT (most sensitive) grouping of detectors. The term P3/P2 (ratio of triples to doubles) is a unique signature of a spontaneous fission isotope. Three of the waste drums depicted in the table indicate P3/P2 values similar to that of <sup>252</sup>Cf and thus contain appreciable amounts of that isotope. Drum 1798 has a low P3/P2 value and therefore probably contains <sup>240</sup>Pu or <sup>242</sup>Pu.

Table 4. ORNL TRU waste drum neutron multiplicity data

Drum/source	neutrons/second	P3/P2	P1/P2
$^{252}\text{Cf}$	900	$0.107 \pm 0.004$	$5.9 \pm 0.1$
2021	$1.6 \times 10^3$	$0.098 \pm 0.004$	$7.9 \pm 0.1$
1925	$1.5 \times 10^2$	$0.078 \pm 0.008$	$10.2 \pm 0.4$
1947	$2.3 \times 10^2$	$0.090 \pm 0.008$	$14.2 \pm 0.6$
1798	$1.7 \times 10^3$	$0.056 \pm 0.008$	$27 \pm 1$
1960	$1.3 \times 10^3$	$0.086 \pm 0.018$	$88 \pm 8$

The P1/P2 ratio (ratio of singles to doubles) is a sensitive function of the relative nonspontaneous fission neutron source content. Drum 1960's P1/P2 value indicates an excess of nonspontaneous fission TRU isotopes relative to spontaneous fission TRU isotopes.

## REFERENCES

1. Management of Transuranic Contaminated Material, DOE Order 5820.1 (Draft OR RWMP #D-1), September 1982.
2. W. E. Kunz et al., A 1-mg-Sensitivity Fissile Assay System, LA-UR-81-1358, Los Alamos National Laboratory, 1981.
3. W. E. Kunz and J. T. Caldwell, Current Status of the Multi-Isotopic Transuranic Waste Assay System, LA-UR-82-787, Los Alamos National Laboratory, April 1982.
4. J. T. Caldwell et.al., Test and Evaluation of a High-Sensitivity Transuranic Waste Assay System, LA-UR-83-377, Los Alamos National Laboratory, in publication.