



Received by [unclear]  
MAY 30 1990

# Lawrence Berkeley Laboratory

UNIVERSITY OF CALIFORNIA

## Materials & Chemical Sciences Division

Presented at the SPIE Superconductivity Applications  
for Infrared and Microwave Devices  
Orlando, FL, April 19–20, 1990, and  
to be published in the Proceedings

### Fabrication of a High $T_c$ Superconducting Bolometer

S. Verghese, P.L. Richards, K. Char, and S.A. Sachtjen

April 1990

DO NOT MICROFILM  
COVER



## **DISCLAIMER**

**This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.**

---

## **DISCLAIMER**

**Portions of this document may be illegible in electronic image products. Images are produced from the best available original document.**

### **DISCLAIMER**

This document was prepared as an account of work sponsored by the United States Government. Neither the United States Government nor any agency thereof, nor The Regents of the University of California, nor any of their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial products process, or service by its trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof, or The Regents of the University of California. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof or The Regents of the University of California and shall not be used for advertising or product endorsement purposes.

Lawrence Berkeley Laboratory is an equal opportunity employer.

LBL--28885

DE90 011306

Fabrication of a High  $T_c$  Superconducting Bolometer

S. Verghese and P.L. Richards

Department of Physics  
University of California

and

Materials and Chemical Sciences Division  
Lawrence Berkeley Laboratory  
University of California  
Berkeley, CA 94720

and

K. Char and S.A. Sachtjen

Conductus Inc.  
Sunnyvale, CA 94086

This work was supported in part by the Director, Office of Energy Research, Office of Basic Energy Sciences, Materials Sciences Division of the U.S. Department of Energy under Contract No. DE-AC03-76SF00098.

*dk*  
DISTRIBUTION OF THIS DOCUMENT IS UNLIMITED

**MASTER**

## Fabrication of a high $T_c$ superconducting bolometer

S. Verghese and P.L. Richards

Dept. of Physics, University of California and Materials  
and Chemical Sciences Division, Lawrence Berkeley Laboratory,  
Berkeley, CA 94720.

K. Char and S.A. Sachtjen

Conductus Inc., Sunnyvale CA 94086.

### ABSTRACT

A sensitive high  $T_c$  superconducting bolometer has been fabricated with a YBCO thin film thermometer on a  $20\mu\text{m}$  thick sapphire substrate. Electrical measurements showed no noticeable film degradation after bolometer fabrication. Optical measurements gave a noise equivalent power of  $5 \cdot 10^{-11} \text{ W/Hz}^{1/2}$  at 10 Hz and a responsivity of 22 V/W. This performance is comparable to that of the very best pyroelectric detectors. Significant improvement appears possible.

### 1. INTRODUCTION

The sensitivity of infrared detectors that operate above liquid  $^4\text{He}$  (LHe) temperatures degrades with increasing wavelength. For wavelengths  $\leq 20\mu\text{m}$  conventional liquid nitrogen-cooled (LN) photovoltaic infrared detectors such as HgCdTe are widely used. For longer wavelengths, however, there is no satisfactory cooled detector technology above LHe temperatures, and room temperature detectors such as Golay cells or pyroelectric detectors are used. A bolometer which operates at the transition temperature of a high  $T_c$  superconductor may offer greater sensitivity at these longer wavelengths<sup>1,2</sup>. This paper describes the design, fabrication, and evaluation of such a bolometer based on epitaxial  $\text{YBa}_2\text{Cu}_3\text{O}_7$  (YBCO) on a  $20\mu\text{m}$  thick  $\text{Al}_2\text{O}_3$  substrate.

## 2. THEORY AND DESIGN

A bolometer consists of a radiation absorber with an electrical resistance thermometer coupled to a heat sink via a thermal conductance. The minimum heat capacity  $C$  is limited by materials consideration. The minimum thermal conductance  $G$  to the heat sink is limited by the background power loading and by the response time  $\tau = C/G$ . The responsivity for a signal modulated at angular frequency  $\omega$  can be written as

$$S(\omega) = I \frac{dR(T)}{dT} |G + i\omega C|^{-1} = \frac{IR}{G\delta T(1 + \omega^2\tau^2)^{1/2}},$$

where  $\delta T$  is half the transition width and  $R$  is the resistance at the operating point near the midpoint of the transition. We neglect the effects of the positive thermal feedback from the current bias which reduces the thermal conductance to an effective value  $G - I^2R/\delta T$ . To maintain thermal stability we arbitrarily constrain the current by the condition  $I^2R \leq 0.3G\delta T$ .

The noise equivalent power (NEP) is calculated by summing the important sources of incoherent noise in quadrature.

$$NEP = \left[ 4kT_c^2G + \frac{4kT_cR}{|S|^2} + \frac{e_n^2 + (i_nR)^2}{|S|^2} + \frac{V_{1/f}^2}{|S|^2} \right]^{1/2}.$$

Ideally, the dominant contributions of a fully optimized bolometer are the first and second terms, phonon shot noise and Johnson noise respectively. Parameters for an optimized bolometer are determined by equating these two contributions. The contribution of the last two terms, amplifier noise and 1/f noise in the high  $T_c$  film respectively, should be smaller in a well designed bolometer. A high  $T_c$  bolometer on a  $1 \times 1 \times 0.02$  mm<sup>3</sup> Al<sub>2</sub>O<sub>3</sub> substrate with  $\delta T = 0.5$  K and  $\omega/2\pi = 10$  Hz could have an NEP  $\approx 10^{-11}$  W/Hz<sup>1/2</sup>. For comparison, a pyroelectric detector<sup>3</sup> optimized for 10 Hz operation has NEP  $\approx 1-5 \cdot 10^{-10}$  W/Hz<sup>1/2</sup>.

## 3. CONSTRUCTION

We chose sapphire as a bolometer substrate for its high Debye temperature and strength. Earlier work<sup>4</sup> indicated high quality c-axis films could be grown directly on  $\{\bar{1}012\}$  Al<sub>2</sub>O<sub>3</sub> by laser ablation. When current biased, these films have excess noise at the resistive transition. The best bolometer made from such films had NEP  $\approx 5 \cdot 10^{-9}$  W/Hz<sup>1/2</sup> at 10 Hz. Films without this excess noise were obtained by *in situ* laser ablation of 3000Å of YBCO on top of a 500Å thick buffer layer of SrTiO<sub>3</sub> on the Al<sub>2</sub>O<sub>3</sub> substrate. The

$6 \times 6 \text{ mm}^2$  chip was then waxed face down to a polishing block and lapped to  $20 \mu\text{m}$  thickness. Electrical contact pads were made by sputter cleaning the YBCO surface in a 1:5  $\text{O}_2 + \text{Ar}$  background and then sputter depositing  $2000 \text{ \AA}$  of Ag. The chip was diced into  $1 \times 1 \text{ mm}^2$  bolometer chips and finally the contacts were annealed in  $\text{O}_2$  at  $500^\circ\text{C}$  for 1 hr.

Electrical leads of  $25 \mu\text{m}$  diameter copper wire were attached to the two silver contact pads with Ag paint. The bolometer chip was suspended by the electrical leads in a temperature regulated brass ring. The bolometer assembly was then mounted on the cold plate of an optical cryostat for electrical and optical characterization.

#### 4. MEASUREMENTS

The bolometer responsivity was directly measured by comparison with a commercial pyroelectric detector and was also calculated from electrical measurements. Figure 1 shows the resistive transition of the completed bolometer for a 1mA current bias. Comparison with measurements made immediately after YBCO deposition showed no noticeable degradation. The steepest part

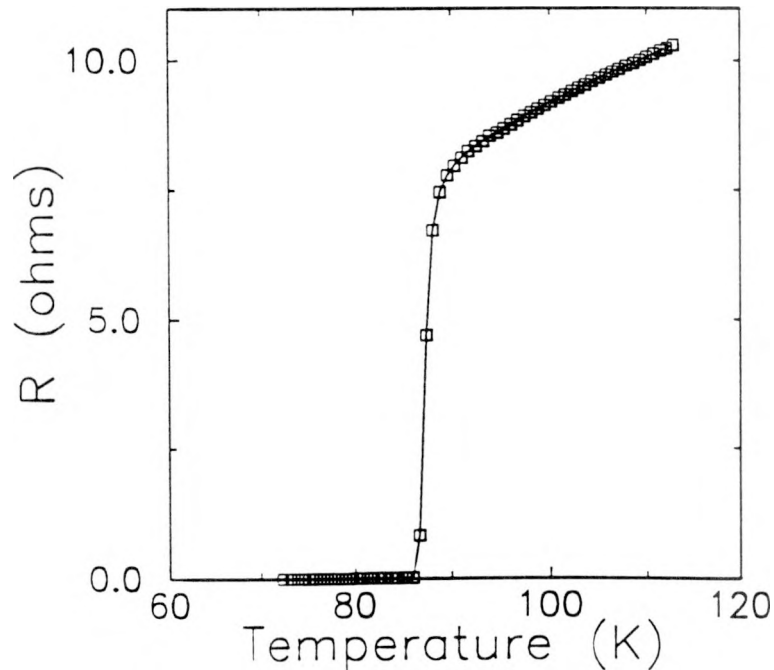


Figure 1: Resistance versus temperature for the bolometer measured at 1mA. This curve was not noticeably degraded by bolometer fabrication.

of the resistive transition has a slope  $dR/dT = 6.2 \Omega/K$  where  $R = 3\Omega$ . Figure 2 shows the dependence of the bolometer resistance on electrical heating by the bias current. We checked that the non-linearity was from heating and found that the film was ohmic at constant temperature. The thermal conductance  $G = 270 \mu W/K$  was obtained from the slope at small  $I^2R$  and from  $R(T)$ .

The bolometer time constant  $\tau = 55$  msec was obtained by measuring the roll off as a function of chopping frequency. We infer a value  $C = 15 \mu J/K$  from the measured values of  $G$  and  $\tau$ . This value is consistent with the computed value  $C = 12 \mu J/K$  and gives us confidence in the  $G$  calculated from Figure 2. From the measured values of  $G$ ,  $dR/dT$ , and  $\tau$ , we calculate a responsivity of 26 V/W at 10Hz and  $I = 4$ mA.

The spectral response of the bolometer is determined by the radiation absorber attached to it. For simplicity, we used the YBCO film as the absorber of 632 nm He-Ne laser light. Figure 3 compares the response to chopped laser light with the slope of the resistive transition. These data are consistent with bolometric response. The peak signal corresponds to an optical responsivity of 22 V/W.

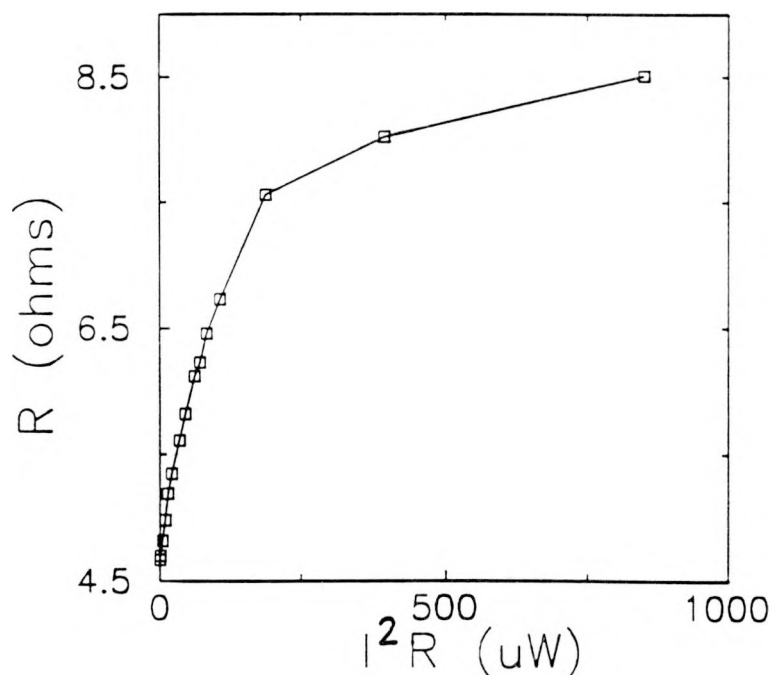


Figure 2: Resistance of the bolometer as a function of electrical heating from the bias current. The nonlinearity of this curve is from the temperature rise and the shape of  $R(T)$ .

We measured the voltage noise in the film for current biases up to 4mA. The excess  $1/f$  noise was so small that we were limited by the  $1.2 \text{ nV/Hz}^{1/2}$  voltage noise in our bipolar amplifier at 10Hz. Using the measured noise we compute optical NEP =  $5 \cdot 10^{-11} \text{ W/Hz}^{1/2}$ . At the maximum current allowed by the stability condition ( $I = 4\text{mA}$ ), the excess  $1/f$  noise in the film was still below amplifier noise. Assuming that the excess noise stays less than Johnson noise, the NEP and responsivity could be improved to  $10^{-11} \text{ W/Hz}^{1/2}$  and 110 V/W at 10Hz by increasing the resistance  $R$  to at least  $200 \Omega$ . This could be done by patterning a meander strip in the YBCO film.

We have designed, fabricated, and tested the first high  $T_c$  bolometer with higher sensitivity than competing room temperature detectors. At a 10 Hz chopping frequency, the lowest NEP is  $5 \cdot 10^{-11} \text{ W/Hz}^{1/2}$  and the responsivity is 22 V/W. Matching the film resistance to the amplifier should further increase the bolometer's sensitivity.

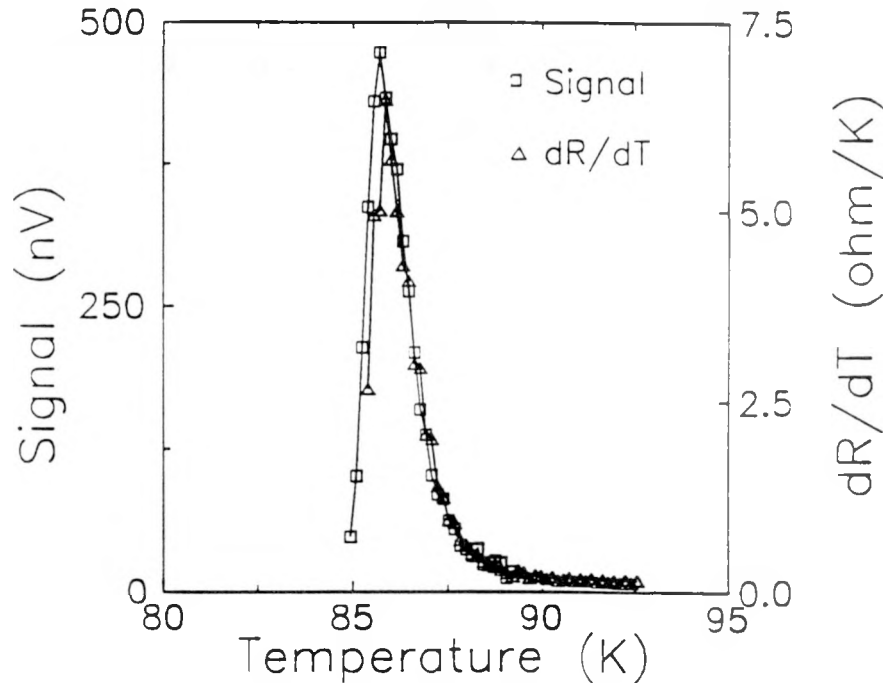


Figure 3: Voltage response of the bolometer to chopped laser light and  $dR/dT$ . The shape of the two curves indicates that the response is bolometric.

## 5. ACKNOWLEDGMENTS

This work was supported in part by the Director, Office of Energy Research, Office of Basic Energy Sciences, Materials Sciences Division of the U.S. Department of Energy under Contract No. DE-AC03-76SF00098 and also by Conductus Inc. S. Verghese acknowledges a Department of Education predoctoral fellowship.

## 6. REFERENCES

1. P.L. Richards, J. Clarke, R. Leoni, Ph. Lerch, S. Verghese, M.R. Beasley, T.H. Geballe, R.H. Hammond, P. Rosenthal, S.R. Spielman, "Feasibility of the high  $T_c$  superconducting bolometer." *Appl. Phys. Lett.* **54**, 283, (1989).
2. P.L. Richards, S. Verghese, T.H. Geballe, S.R. Spielman, "The high  $T_c$  superconducting bolometer." 1988 Applied Superconductivity Conference. *IEEE Trans. Magn.* **MAG-25**, 1335, (1988).
3. See, for example the P-41 detector, Molelectron Corp., Sunnyvale, CA.
4. K.Char, D.K. Fork, T.H. Geballe, S.S. Laderman, R.C. Taber, R.D. Jacowitz, F. Bridges, G.A.N. Connell, J.B. Boyce, "Properties of epitaxial  $YBa_2Cu_3O_7$  thin films on  $Al_2O_3$   $\{\bar{1}012\}$ ," *Appl. Phys. Lett.* **56**, 785, (1990).