

RECEIVED
JAN 18 2000
OSTI

Atom Trap Trace Analysis of Krypton Isotopes

K. Bailey,¹ C.Y. Chen,¹ X. Du,¹ Y.M. Li,¹ Z.-T. Lu,¹ T.P. O'Connor,¹ L. Young²

¹Physics Division, ²Chemistry Division, Argonne National Laboratory,
9700 South Cass Avenue, Argonne, IL 60439, USA

Abstract: A new method of ultrasensitive isotope trace analysis has been developed. This method, based on the technique of laser manipulation of neutral atoms, has been used to count individual ⁸⁵Kr and ⁸¹Kr atoms present in a natural krypton gas sample with isotopic abundances in the range of 10^{-11} and 10^{-13} , respectively. This method is free of contamination from other isotopes and elements and can be applied to several different isotope tracers for a wide range of applications. The demonstrated detection efficiency is 1×10^{-7} . System improvements could increase the efficiency by many orders of magnitude.

We report a new atom-counting method, named Atom Trap Trace Analysis (ATTA) [1]. This method is based on laser manipulation of neutral atoms, and has been successfully applied to count ⁸⁵Kr and ⁸¹Kr (Table 1) in natural krypton samples. ATTA differs significantly from all previous methods in that it is free of any contamination from different isotopes or elements. Therefore, ATTA can tolerate impure gas samples, does not require a special operation environment, and its apparatus can be made transportable for applications that require on-site analysis.

Our design (Fig. 1) is based on a type of magneto-optical trap system that had been used to trap various metastable noble gas atoms [2]. Trapping krypton atoms in the $5s[3/2]_2$ metastable level (lifetime = 40 sec) is accomplished by exciting the $5s[3/2]_2 - 5p[5/2]_3$ transition using laser light with a wavelength of 811 nm generated by a Ti:Sapphire ring laser. The laser frequency, after shifting by acousto-optical modulators (AOM) to account for the isotope shift, is locked to a reference absorption line of the abundant ⁸³Kr atoms in a cell. Krypton gas sample is injected into the system through a 0.1 mm diameter nozzle, around which a DC discharge is maintained. A fraction, about 1×10^{-4} , of the atoms are excited into the $5s[3/2]_2$ level by the discharge and, after exiting the discharge region, remain in this metastable level until they hit walls. Two-dimensional transverse cooling is used to reduce the atomic beam divergence and amplify the atom flux in the forward direction by a factor of 20. The thermal (300°C) atoms are then decelerated with the Zeeman slowing technique [3], and loaded into a magneto-optical trap [4]. Atoms remain trapped for an average of 1.8 sec when the vacuum is maintained at 2×10^{-8} Torr. This trap system can capture the abundant ⁸³Kr (isotopic abundance = 11.5%) atoms at the rate of $2 \times 10^8 \text{ sec}^{-1}$. The ratio of the capture rate to the injection rate gives a total capture efficiency of 1×10^{-7} .

DISCLAIMER

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, make any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.

DISCLAIMER

Portions of this document may be illegible in electronic image products. Images are produced from the best available original document.

In the trap, a single atom scatters resonant photons at a rate of 10^7 sec^{-1} , of which 1% are collected, spatially filtered to reduce background light, and then focused onto an avalanche photodiode (EG&G, SPCM-AQ-212) with a specified photon counting efficiency of 25%. For single atom detection, each trapping laser beam is set at 1 cm diameter and 2 mW/cm^2 , and the magnetic field gradient of the MOT set at 16 G/cm along its axis. Under these conditions, fluorescence from a single atom induces a signal of 16 kilo-counts per second (kcps) while the background level is 3.4 kcps (Fig. 2). These laser and field parameters differ significantly from those needed for an optimum trap loading rate (3 cm diameter, 10 mW/cm^2 , and 8 G/cm field gradient). The trap loading conditions generate too much background light to permit single atom detection so we switch at about 2 Hz between the optimal parameters for loading and detection.

We have trapped and counted ^{85}Kr and ^{81}Kr atoms from natural krypton gas (Fig. 2). The frequency settings of the trapping laser are in good agreement with previous spectroscopic measurements obtained using enriched ^{85}Kr gas and enriched ^{81}Kr gas [5]. We mapped the atom capture rate versus laser frequency (Fig. 3), and showed that the maximum loading was achieved with the frequency detuned approximately 4 MHz below resonance, consistent with the results observed on ^{83}Kr traps (Fig. 3a). Furthermore, repeated tests were performed under conditions in which a ^{85}Kr (^{81}Kr) trap should not work, such as tuning the laser frequency above resonance, and these tests have always yielded zero atom counts. These tests show that the recorded counts are due to laser-trapped ^{85}Kr (^{81}Kr) atoms, and that no background atom-counts from other isotopes or elements have been observed.

Previous efforts to develop a laser-based technique have encountered serious problems with contamination from nearby abundant isotopes. ATTA is immune from isotope contamination for several reasons: fluorescence is only collected in a small region (0.5 mm diameter) around the trap center; a trapped atom is cooled to a speed below 1 m/s so that its laser induced fluorescence is virtually Doppler-free; a trapped atom allows a long observation time, during which 10^3 scattered signal photons are collected; and trapping allows the temporal separation of capture and detection so that both capture efficiency and detection sensitivity can be optimized. With a 100 ms observation period, the signal of a single trapped atom is 50 times the noise (1σ) of the background photons.

Besides isotopic selectivity, another important characteristic is detection efficiency. The efficiency of our system depends on the discharge current, laser power, as well as optical alignment. At one particular setting, we measured capture rates of ^{83}Kr , ^{85}Kr , and ^{81}Kr , which were $(1.5 \pm 0.3) \times 10^8 \text{ sec}^{-1}$, $(1.9 \pm 0.3) \times 10^2 \text{ sec}^{-1}$, and $(1.3 \pm 0.4) \times 10^{-3} \text{ sec}^{-1}$, respectively. If we assume the same detection efficiency for all three isotopes, then we get isotopic abundances of $(1.5 \pm 0.4) \times 10^{-11}$ for ^{85}Kr and $(1.0 \pm 0.4) \times 10^{-12}$ for ^{81}Kr , which are in good agreement with previous measurements using other methods [6, 7, 8]. The capture efficiencies can be calibrated with enriched samples of known isotopic abundance to correct for any isotope-dependent effects and measure isotopic ratios in unknown samples.

Our system has achieved an efficiency of 1×10^{-7} , which limits the current system to atmospheric applications where large samples of gas are readily available. It is possible to raise the efficiency many orders of magnitude through improvements such as cryogenic cooling in the discharge region

and re-circulation of krypton gas. Another promising way to improve efficiency is to use an ultra-violet (UV) laser to excite the atoms to the metastable level via a two-photon transition. In one proposed scheme, krypton atoms are excited by a CW-laser ($\lambda = 216\text{nm}$) from the ground-level to the $5p[3/2]_2$ excited-level, from which about 10% of these atoms decay into the $5s[3/2]_2$ metastable level. We calculate [9] that 5% of the atoms can be transferred to the $5s[3/2]_2$ level in an arrangement where atoms cross an intense laser beam (10 Watts over $100\mu\text{m}^2$) present at the center of a near-concentric power build-up cavity. Without the constraint from the discharge, the atoms can be collimated and cooled to liquid nitrogen temperature, thus further reducing the loss due to beam divergence. This scheme should improve the detection efficiency to about 10^{-3} . Further improvement is possible if the krypton atoms are recycled back to the source. Another proposal seeks to combine the high efficiency of the "atom buncher" [10] and the high selectivity of ATTA. In this scheme, krypton atoms are collected to a cold spot cooled by liquid helium inside an enclosed cell. A pulse of laser light is directed to the cold spot to release some atoms at low temperature. This is followed by another UV-laser pulse to excite the released atoms to the $5s[3/2]_2$ level. The metastable atoms of interest are then captured into a trap.

ATTA can be applied to many different isotopes. Laser trapping is well established on alkali, alkali earth, and noble gas elements. Trapping of other elements is generally more difficult due to both the complexity of their ground level structures and the lack of suitable UV lasers. Some of these problems could be overcome with future advances in UV laser technology.

We thank C. Wieman and W. Kutschera for stimulating discussions. This work is supported by the U.S. Department of Energy, Nuclear Physics Division, and LY by the Office of Basic Energy Sciences, Division of Chemical Sciences, under contract W-31-109-ENG-38.

References:

- [1] C.Y. Chen, Y.M. Li, K. Bailey, T.P. O'Connor, L. Young, Z.-T. Lu, *Science* **286**, 1139 (1999).
- [2] M. Walhout, H.J.L. Megens, A. Witte, S.L. Rolston, *Phys. Rev. A* **48**, R879 (1993).
- [3] W. Phillips and H. Metcalf, *Phys. Rev. Lett.* **48**, 596 (1982).
- [4] E.L. Raab, M. Prentiss, A.E. Cable, S. Chu, D.E. Pritchard, *ibid.* **59**, 2631 (1987).
- [5] B.D. Cannon, *Phys. Rev. A* **47**, 1148 (1993).
- [6] *Isotope of Noble Gases as Tracers in Environmental Studies*, International Atomic Energy Agency (IAEA, Vienna, 1992).
- [7] H.H. Loosli and H. Oeschger, *Earth Planet. Sci. Lett.* **7**, 67 (1969).
- [8] P. Collon et. al., *Nucl. Instr. and Meth.* **B123**, 122 (1997).
- [9] A.A. Radzig and B.M. Smirnov, *Reference Data on Atoms, Molecules, and Ions* (Springer-Verlag, New York 1985).
- [10] G.S. Hurst, M.G. Payne, R.C. Phillips, J.W.T. Dabbs, B.E. Lehmann, *J. Appl. Phys.* **55**, 1278 (1984).

Table 1. The properties of ^{85}Kr and ^{81}Kr .

	Half-Life(yr)	Atmospheric isotope abundance	Main production source
^{85}Kr	10.8	$\sim 1 \times 10^{-11}$ (LLC, 6)	A fission product of U and Pu.
^{81}Kr	2.3×10^5	$(5.9 \pm 0.6) \times 10^{-13}$ (LLC, 7) $(5.3 \pm 1.2) \times 10^{-13}$ (AMS, 8)	Cosmic-ray induced spallation and neutron activation of stable Kr.

Figure 1. Schematic diagram of the atom beamline. Total length of the apparatus is about 2.5 meters.

Figure 2. Signal of a single trapped ^{81}Kr atom. During loading time, the photon-count rate was low because the counter was blocked for protection from over-exposure.

Figure 3. (a) Fluorescence of trapped ^{83}Kr atoms vs. laser frequency. Fluorescence was measured with a low-gain photo-diode detector. (b) Number of ^{81}Kr and ^{85}Kr atoms counted vs. laser frequency. Each data point represents the number of atoms counted in 3 hours for ^{81}Kr , and 0.5 hours for ^{85}Kr .

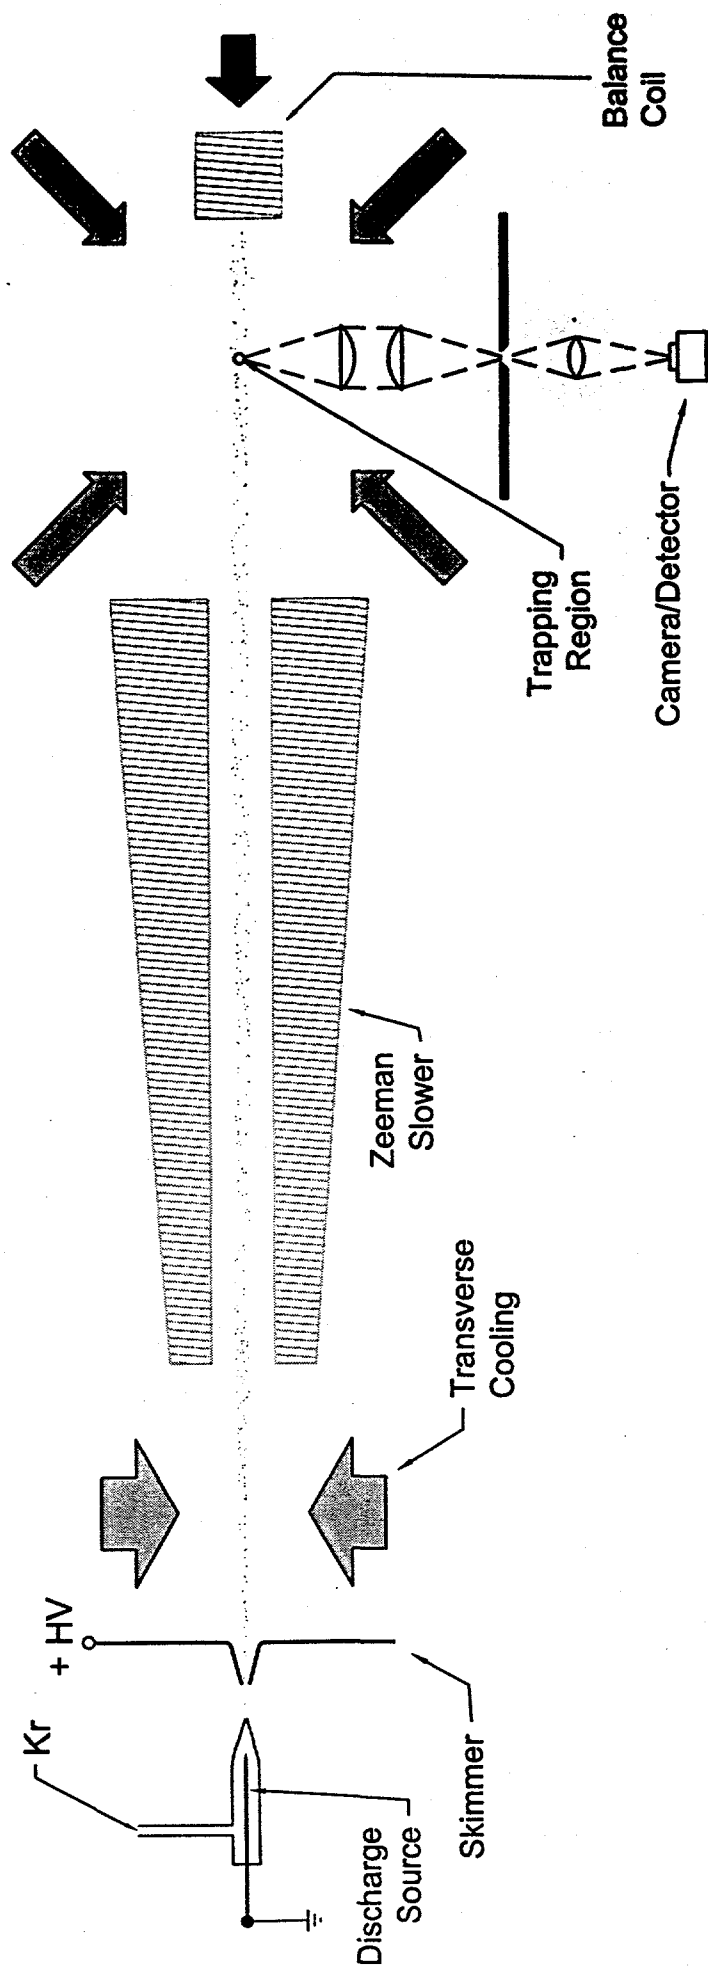


Fig. 1

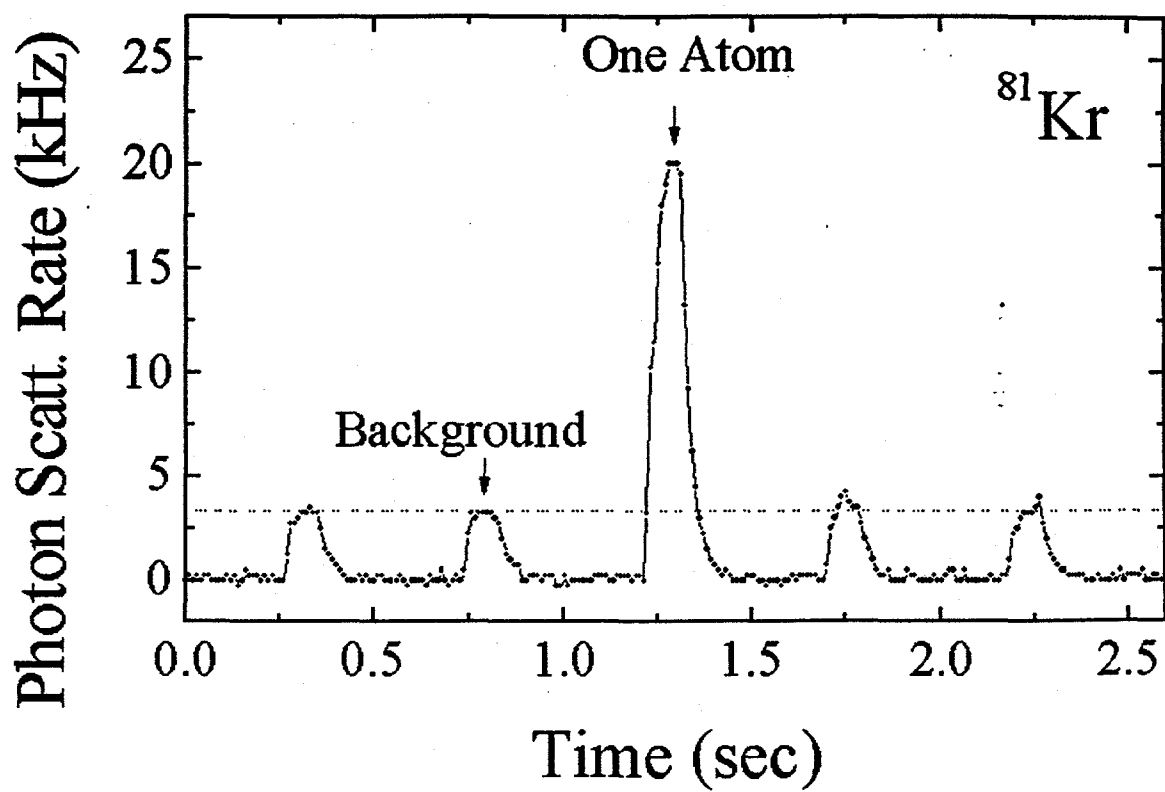


Fig. 2

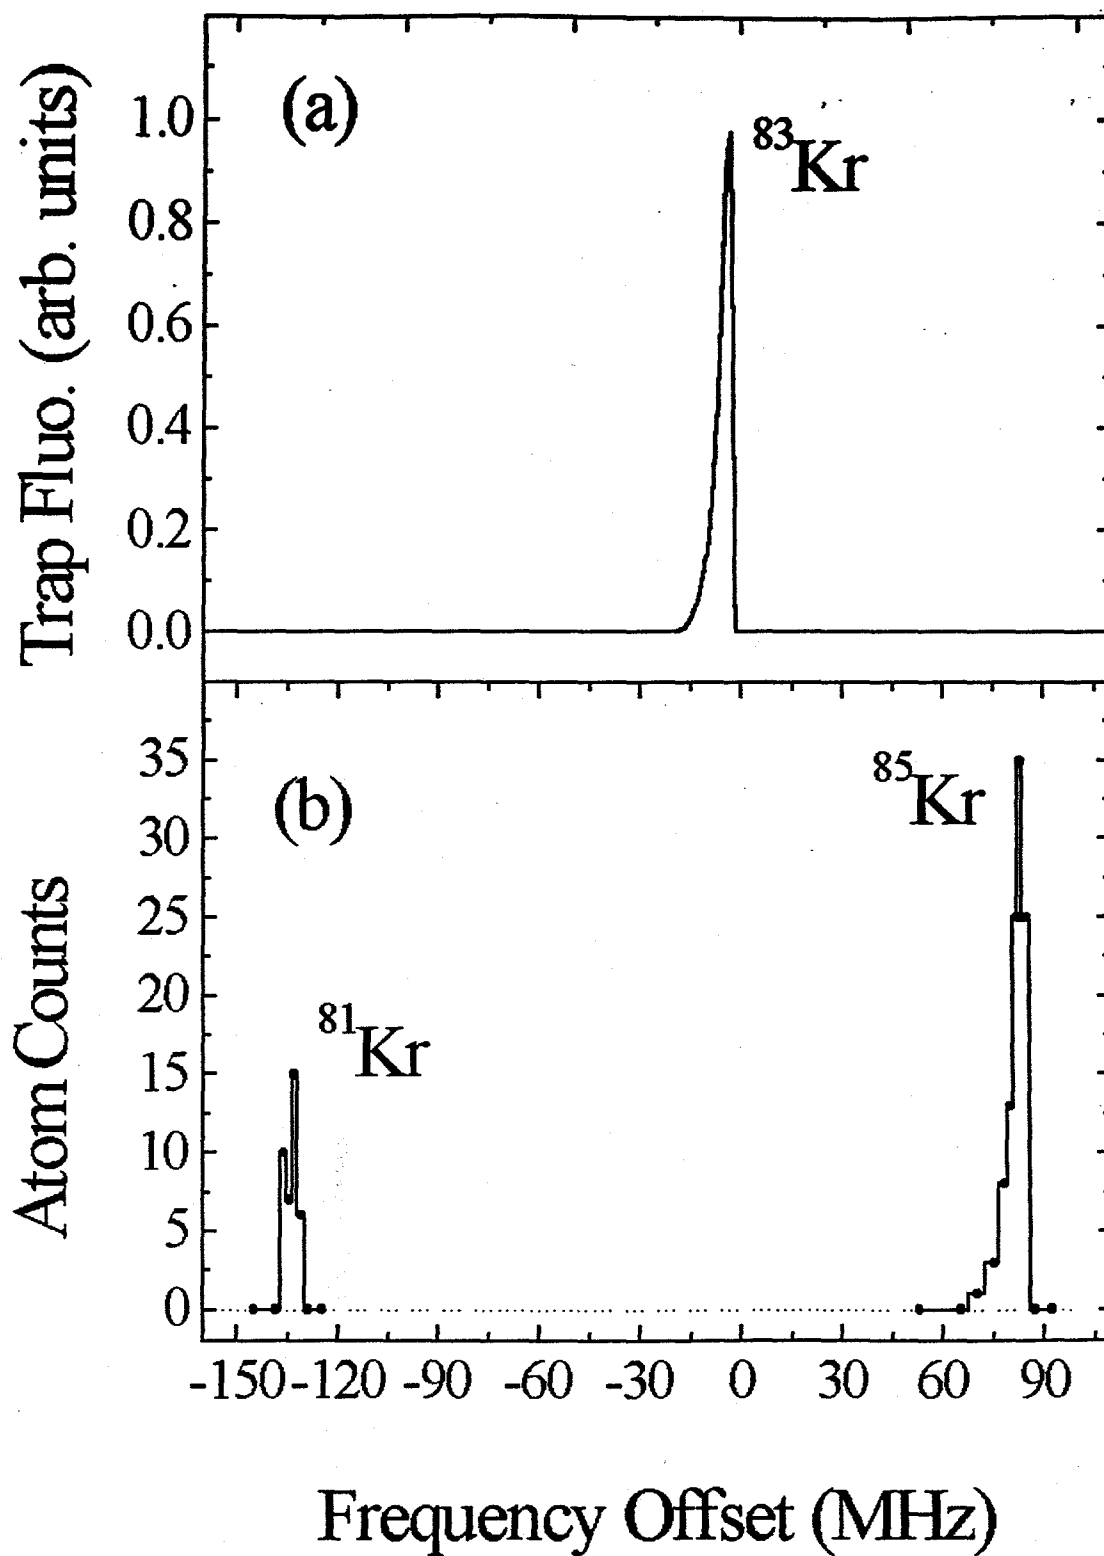


Fig. 3