

# Laser Ablation-Inductively Coupled Plasma-Atomic Emission Spectroscopy Study at the 222-S Laboratory Using Hot-Cell Glove Box Prototype System

**C. M. Seidel, J. Jain, and J. W. Owens**  
Washington River Protection Solutions LLCC  
Richland, WA 99352  
U.S. Department of Energy Contract DE-AC27-08RV14800

EDT/ECN: DRF UC:  
Cost Center: Charge Code: 2EK00  
B&R Code: Total Pages: 644 including DRF and this page  
34 02 23 09

**Key Words:** Laser Ablation, Task Order 2005-003, LA-ICP-AES, Waste Treatment and Immobilization Plant;

**Abstract:** This report describes the installation, testing, and acceptance of the Waste Treatment and Immobilization Plant (WTP) procured laser ablation-inductively coupled plasma-atomic emission spectroscopy (LA-ICP-AES) system for remotely analyzing high-level waste (HLW) samples in a hot cell environment. The work was completed by the Analytical Process Development (APD) group in accordance with Task Order 2005-003; ATS MP 1027, Management Plan for Waste Treatment Plant Project Work Performed by Analytical Technical Services. The APD group at the 222-S Laboratory demonstrated acceptable turnaround time (TAT) and provide sufficient data to assess sensitivity, accuracy, and precision of the LA-ICP-AES method.

TRADEMARK DISCLAIMER. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof or its contractors or subcontractors.

Release Approval

2/23/2009  
Date

Date



---

Release Stamp

Approved For Public Release

# **Laser Ablation-Inductively Coupled Plasma-Atomic Emission Spectroscopy Study at the 222-S Laboratory Using Hot-Cell Glove Box Prototype System**

Washington River Protection Solutions LLC

Date Published  
February 2009



Prepared for the U.S. Department of Energy  
Office of River Protection

Contract No. DE-AC27-08RV14800

## EXECUTIVE SUMMARY

This report describes the installation, testing, and acceptance of the Waste Treatment and Immobilization Plant (WTP) procured laser ablation-inductively coupled plasma-atomic emission spectroscopy (LA-ICP-AES) system for remotely analyzing high-level waste (HLW) samples in a hot cell environment. The method tested in this study was developed through a team effort at Savannah River National laboratory (SRNL) (WSRC-TR-2005-00260, *The Development of Laser Ablation-Inductively Coupled Plasma-Atomic Emission Spectroscopy for the Analysis of Hanford High Level Waste*), and Pacific Northwest National laboratory (WTP-RPT-140, *Laser Ablation/ICP-AES Time Study*). The work was completed by the Analytical Process Development (APD) group in accordance with the task plan (Appendix A) that addresses the scope defined by Memorandum of Agreement CHG-BNI-2001; Task Order 2005-003; ATS-MP-1027, *Management Plan for Waste Treatment Plant Project Work Performed by Analytical Technical Services*, as directed by statement of work authorized by Bechtel National, Inc. The APD group at the 222-S Laboratory was requested to demonstrate acceptable turnaround time (TAT) and provide sufficient data to assess sensitivity, accuracy, and precision of the LA-ICP-AES method.

This work began with the APD assisting WTP in the procurement of the prototype LA-ICP-AES glove box system and subsequent installation in the hot cell facility of the 222-S Laboratory. The system was tested for operability prior to initiating the analytical work specified in the task plan (Appendix A). The LA-ICP-AES was calibrated using the known glass coupons that were prepared and characterized at SRNL.

Scoping tests were performed on a radioactive AY-102 sample that was prepared at SRNL by vitrifying the HLW slurry into a glass coupon. The sample was analyzed for 23 elements (Al, B, Ca, Cd, Cr, Fe, K, Li, Mg, Mn, Na, Ni, P, S, Sb, Si, Sr, Th, Ti, Tl, U, Zn, and Zr). Lithium borate glass was included as a blank and an analytical reference glass (ARG-1) was analyzed as a laboratory control sample for each batch of samples.

Under carefully designed experimental conditions, a sufficient accuracy and precision was demonstrated. The precision of analysis for most of the elements was ~5% relative standard deviation. The accuracy of the analysis was compared within  $\pm 15\%$  of the wet chemistry analysis results for 10 elements (Al, B, Ca, Fe, Li, Mg, Na, Ni, Si, and Ti) for a Hanford tank waste sample from 241-AY-102/C-106 (AY-102). The comparisons for P, Mn, Zn, and Cr were higher than the 10 elements above. Elements Cd, K, Sr, Zr, and Sb were not detected because of their low abundance in the AY-102 sample. The accuracy of S cannot be assessed because of the uncertainty in the reported value. Due to the lack of sufficient calibration data for Th, Tl, and U, the data for these elements should be considered qualitative. The TAT study evaluated total time required from sample preparation (conversion of sludge to a glass puck) to data reduction. The sample preparation time was less than 2 hours. The TAT for sample analysis included two process batches: one batch of four AY-102 samples and another batch of eight AY-102 samples. Both batches included blank and quality control samples. The analysis time for both batches was less than 5 hours. Data reduction was completed in less than 2 hours. The TAT from receipt of

sample, sample preparation, and data processing was shown to be less than 9 hours for each batch.

The results obtained from the analysis of the radioactive AY-102 glass are satisfactory. The adaptation of the developed method (for hot cell testing using radioactive samples) successfully demonstrated the acceptance of the selected technology for meeting the rapid TAT requirements for monitoring the vitrification process. The LA-ICP-AES results were verified with wet chemistry data. The waste generated from the LA-ICP-AES method is significantly less when compared to conventional dissolution methods.

## Table of Contents

EXECUTIVE SUMMARY .....	i
LIST OF ACRONYMS .....	v
1. INTRODUCTION AND BACKGROUND .....	1
2. INSTALLATION AND ACCEPTANCE.....	2
3. ANALYTICAL TESTING .....	3
3.1    DEVELOPMENT AND OPTIMIZATION OF THE GLASS FUSION SAMPLE PREPARATION.....	3
3.2    LA-ICP-AES TEST PARAMETERS AND ANALYSIS .....	4
3.2.1    Laser Optimization.....	6
3.2.2    Inductively Coupled Plasma-Atomic Emission Spectroscopy Parameters .....	8
3.2.3    Inductively Coupled Plasma-Atomic Emission Spectroscopy Emission Lines .....	8
3.2.4    Particle Trap .....	9
3.2.5    Sample Analysis.....	10
3.2.6    Internal Standard .....	10
3.2.7    Instrument Calibration.....	11
3.2.8    Detection Limits .....	13
3.2.9    Radioactive Glass Sample and Analysis Sequence.....	14
3.2.10    Precision and Accuracy.....	15
3.2.11    Operator and Day Variability.....	18
3.2.12    Turnaround Time Study .....	18
3.2.13    Analysis of 241-AN-102 .....	21
4. QUALITY ASSURANCE AND SAFETY .....	21
5. DISCUSSION AND RECOMMENDATIONS.....	23
6. REFERENCES .....	24

## Appendices

**NOTE: Appendixes A through H are for Official Use Only (OUO) and are not included with this report but can be accessed through the OUO process.**

APPENDIX A	Waste Treatment and Immobilization Plant/222-S Laser Ablation Task Plan; CH2M-0600207 REISSUE.....	A-i
APPENDIX B	Hold Points Defined in the Waste Treatment and Immobilization Plant/222-S Laser Ablation Task Plan (CH2M-0600207).....	B-i
APPENDIX C	Waste Treatment and Immobilization Plant Certificate of Conformance.....	C-i
APPENDIX D	Photographs of System Installation .....	D-i
APPENDIX E	Work Package for LA-ICP-AES Installation (step 1 and step 2) .....	E-i
APPENDIX F	General LA-ICP-AES Analytical Procedure ATS-LT-505-105 .....	F-i

APPENDIX G	General Operation and Maintenance Procedure ATS-LO-161-183 .....	G-i
APPENDIX H	Copy of LA-ICP-AES Data Printouts.....	H-i

### **List of Figures**

Figure 1. Shipping Damage to Assembly Bolts on Bottom of Glove Box.....	2
---	---

### **List of Tables**

Table 1. Sequential Steps for Preparing Glass Coupons in 11A3 Hot Cell.....	4
Table 2. Consensus-Value Composition (wt%) of ARG-1 and SRM 610 .....	5
Table 3. Stability of Signal Using Raster Sample Pattern Over Time (SRM 610).....	7
Table 4. Laser Operating Parameters.....	7
Table 5. Inductively Coupled Plasma-Atomic Emission Spectroscopy Operating Parameters....	8
Table 6. Inductively Coupled Plasma-Atomic Emission Spectroscopy Wavelength Selection ....	9
Table 7. Effect of Particle Trap on the Precision of Analysis .....	9
Table 8. Precision of Analysis of AY-102.....	11
Table 9. Composition of Glass Standards (wt%).....	12
Table 10. Coefficients of Regression ( $r^2$ ) from Calibration Curves .....	13
Table 11. Estimated Detection Limits .....	14
Table 12. Reported and Analyzed Concentrations (wt%) in ARG-1 Glass Coupon .....	16
Table 13. Analyzed and Reported Elemental Concentrations (wt%) in AY-102 Glass Coupon	17
Table 14. Analyzed and Reported Concentrations (wt%) of Th, Tl, and U in AY-102 Glass ....	18
Table 15. Elemental Concentration (wt%) of AY-102 Analyzed by Different Operators on Different Days .....	19
Table 16. Turnaround Time Study.....	20
Table 17. LA-ICP-AES and ICP-AES Method Comparison (wt%).....	22

## LIST OF ACRONYMS

APD	Analytical Process Development
ARG-1	Analytical Reference Glass (ARG-1 “Glass standard 1”)
ATL	Advanced Technologies and Laboratories International, Inc.
AY-102	Refers to the waste sampled from tank 241-AY-102 after the contents of tank 241-C-106 was transferred to 241-AY-102. Also referred to as 241-AY-102/C-106
HLW	high-level waste
ICP-AES	inductively coupled plasma-atomic emission spectroscopy
LA-ICP-AES	laser ablation-inductively coupled plasma-atomic emission spectroscopy (also referred to as laser ablation inductively coupled plasma atomic emission spectrometry)
LCS	laboratory control sample
PNNL	Pacific Northwest National Laboratory
RSD	relative standard deviation
SRNL	Savannah River National Laboratory
TAT	turnaround time
UV	ultraviolet
WRPS	Washington River Protection Solutions LLC
wt%	weight percent
WTP	Waste Treatment and Immobilization Plant

## 1. INTRODUCTION AND BACKGROUND

This report documents the completion of the study to determine the applicability of laser ablation-inductively coupled plasma-atomic emission spectroscopy (LA-ICP-AES) glove-box technology as a primary process control analytical technique supporting the Hanford Waste Treatment and Immobilization Plant (WTP). The following appendixes are included with this report:

- Appendix A Waste Treatment and Immobilization Plant/222-S Laser Ablation Task Plan; CH2M-0600207 REISSUE
- Appendix B Hold Points Defined in the Waste Treatment and Immobilization Plant/ 222-S Laser Ablation Task Plan (CH2M-0600207)
- Appendix C Waste Treatment and Immobilization Plant Certificate of Conformance
- Appendix D Photographs of System Installation
- Appendix E Work Package for LA-ICP-AES Installation (step 1 and step 2)
- Appendix F General LA-ICP-AES Analytical Procedure ATS-LT-505-105
- Appendix G General Operation and Maintenance Procedure ATS-LO-161-183
- Appendix H Copy of LA-ICP-AES Data Printouts

This task represents Phase II of the WTP method development study following the completion of Phase I (WSRC-TR-2005-00260, *The Development of Laser Ablation-Inductively Coupled Plasma-Atomic Emission Spectroscopy for the Analysis of Hanford High Level Waste: Phase I*, and WTP-RPT-140, *Laser Ablation/ICP-AES Time Study*) for the implementation of the LA-ICP-AES method in the WTP laboratory. This work included investigating the configuration and efficiency of the system for use in the Hanford WTP process support laboratory. This task was completed by Washington River Protection Solutions LLC (WRPS) with the transition to the Tank Operations Contract on October 1, 2008.

Analytical characterization techniques must be robust to process compositional variations and must be capable of meeting the specified sample analytical time available to maintain process design production rates and produce acceptable glass. This investigation was to verify the required sample turnaround time (TAT) of less than 9 hours is achievable using the LA-ICP-AES hot-cell glove-box prototype system on an actual high-level waste (HLW) sample. The method adaptation and testing was studied to determine if LA-ICP-AES technology can provide sufficient accuracy and precision to determine melter feed chemistries.

The work reported here involves (a) installation and testing of a WTP procured LA-ICP-AES glove-box system properly configured in the adjacent hot cell for remotely ablating HLW samples, and (b) adaptation of the Phase I developed LA-ICP-AES method to routine operational requirements. In addition, the adapted Phase I methodology must demonstrate acceptable TAT and meet the requirements of determinative methods for elemental analysis. This work addressed the scope defined by Memorandum of Agreement CHG-BNI-2001; Task


Order 2005-003; ATS-MP-1027, *Management Plan for Waste Treatment Plant Project Work Performed by Analytical Technical Services*, and the associated statement of work. This report covers the task descriptions for system installation, subsequent testing of developed methodology, and establishing TAT for the analytical process. The purpose of the study was to demonstrate the feasibility of implementing the LA-ICP-AES technology for WTP laboratory monitoring of the vitrification process.

## 2. INSTALLATION AND ACCEPTANCE

The installation of the LA-ICP-AES was performed under Work Package 2S-04-02382. A copy of this work package and the supporting documentation is attached in Appendix E step 1 and Appendix E step 2. Step 1 of the work package covers site preparation up to receipt of the LA-ICP-AES from the vendor. Step 2 covers the installation and vendor testing. The development of the site installation work instructions and some site pre-acceptance preparations were conducted prior to receipt of and acceptance of the vendor's equipment. After vendor acceptance testing was conducted at the vendor's facility in Omaha, Nebraska, the equipment was shipped to the WTP Marshaling Yard and then transferred to the 222-S Laboratory on April 8, 2008.

On receipt at the 222-S Laboratory, shipping damage was noted on the assembly bolts on the bottom of the glove box (see Figure 1). As shown in Figure 1, the mounting bolts were bent slightly out of alignment. It was noted that the crating of the glove box allowed the unit to freely float within the shipping crate. At the time of receipt, the damage noted was not severe enough to prevent installation. Later, during installation, additional damage was discovered to the computer table and torch positioning apparatus within the glove box that was not apparent at the loading dock when the equipment was received. While there was no evident damage to the edges of the computer table, the table top was split across the width in the center of the table.

**Figure 1. Shipping Damage to Assembly Bolts on Bottom of Glove Box**

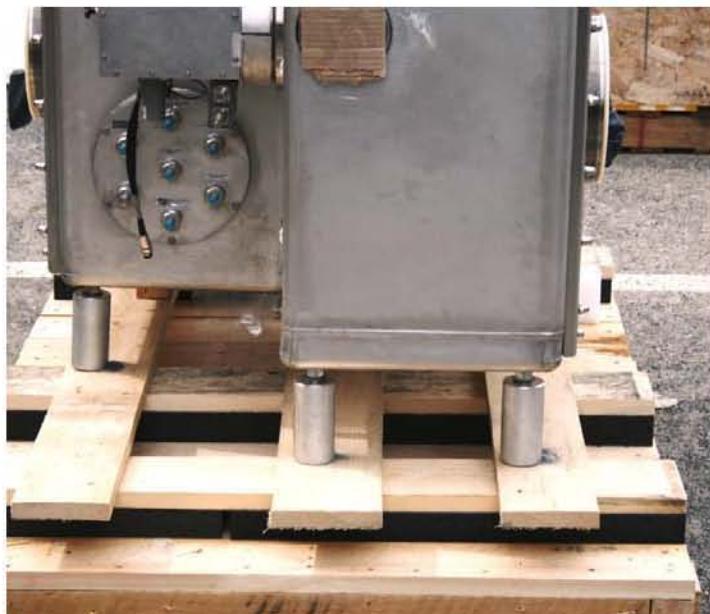

The onsite installation continued immediately on receipt and acceptance of the equipment. Photographs of the installation are attached in Appendix D of this report. The equipment was assembled by the 222-S Facility Maintenance and plant personnel including modifications to utility feeds. No major issues were encountered during installation, although the damage to the torch positioning apparatus delayed the vendor acceptance test while troubleshooting and repair of this part of the LA-ICP-AES was accomplished by the vendor.

### 3. ANALYTICAL TESTING

#### 3.1 DEVELOPMENT AND OPTIMIZATION OF THE GLASS FUSION SAMPLE PREPARATION.

This task included development of a glass fusion procedure that was applicable to the hot cell environment. Glass coupons prepared from tank simulant were produced in accordance with test plan 7S110-MFM-07-096, "Preparation of Glass Coupons from Tank Simulant." Developmental work was performed using "Early Feed Chemical Simulant" identified as FY-06-SS Early. The guidelines for the production of the glass coupons included the following constraints:

- a. Each coupon shall contain less than 3 g of tank waste solids.
- b. Glass formers and temperature shall be achievable in the hot cell environment.
- c. The procedure used would be simple enough to perform remotely.
- d. The fusion of the glass would not produce an unacceptable heat load on the hot cell.

Coupon size consisted of the following:

- a. Diameter: 25 mm–35 mm (optimum 30 mm); smaller sizes can be used with an adapter.
- b. Thickness: 1.6 mm–6 mm (optimum 4 mm).
- c. Broken shards will be usable with an adapter.

Compliance with the above guidelines was achieved. A 1 to 4 ratio of sample and flux was used to prepare the glass coupon. Sample weight used was approximately 1.67 g. Glass coupons measured during the development period produced a coupon thickness from 3.06 mm to 4.36 mm and diameters of 27.52 mm to 30.71 mm.

A borate fusion technique was used to prepare glass coupons in 11A hot cell. A radioactive sample was placed in a crucible and transferred to the muffle furnace at 200 °C to obtain a dried slurry sample. The dried slurry sample was mixed in an approximate 1 to 4 ratio of lithium metaborate/lithium tetraborate flux comprised of 34% lithium metaborate and 66% lithium tetraborate. The mixture was then spiked with germanium oxide as an internal standard. Lithium bromide was added as a non-wetting agent to prevent the flux from sticking to the crucible and mold when removed. The dried radioactive waste sample and flux were then placed in a 95% platinum 5% gold crucible and placed in the muffle furnace at 1100 °C with constant agitation. The 30-mm mold was also placed in the furnace at this time to ensure it was at the

proper temperature to accept the glass once fused. A SK-600 reciprocating shaker set at 60 revolutions per minute for 15 minutes was used to ensure that the sample completely dissolved into the molten flux. After this step was completed, the shaker was turned off; the melt was poured into a heated 30-mm-diameter platinum/gold mold, and allowed to cool to 500 °C in the muffle furnace with the door open prior to placing the glass sample in a desiccator to complete the cooling period. The complete fusion procedure resulted in a TAT of 1 hr 45 minutes. This procedure is fully defined in Appendix F.

Table 1 represents sequential steps and the time taken to prepare a glass coupon in the hot cell. To ensure the procedure was safe in the hot cell environment, thermocouples were placed in the hot cell to monitor the impact of the heat load from this method. The temperature close to the glass windows did not increase more than 1 °C during the performance of this activity.

**Table 1. Sequential Steps for Preparing Glass Coupons in 11A3 Hot Cell**

Step	Preparation Sequence	Duration (minutes)
1	The balance is tared	1
2	A sample weight of slurry and crucible is obtained	3
3	Sample drying at 200 °C	30
4	The crucible is removed from the muffle furnace	1
5	The crucible is cooled for 30 minutes, and the muffle furnace temperature is taken from 200 °C to 1100 °C	30
6	The dried slurry sample, flux, and lithium bromide is placed into the crucible and reweighed (the internal standard is added here)	2
7	The crucible is placed in the furnace for fusion and shaker is started	15
8	The crucible is removed from the furnace and the melt poured into the mold. The furnace door remains open, The furnace is shut off, and the melt allowed to cool to ~500 °C	7
9	At ~400 °C the mold is removed from the muffle furnace	1
10	The mold is placed in the desiccator to cool	15
11	The glass coupon is removed from the mold	
	Total time to prepare glass coupon in hot cell	1 hour 45 minutes

### 3.2 LA-ICP-AES TEST PARAMETERS AND ANALYSIS

The test scope utilized the method developed in parallel studies conducted at Savannah River National Laboratory (SRNL) and Pacific Northwest National Laboratory (PNNL). The instrument model and configurations used in those two studies were different. Therefore the optimization of the LA-ICP-AES prototype system was necessary for reproducible, reliable results. The instrument system optimization was performed using two glass coupons, SRM 610 and ARG-1, which contained a significant number of analytes of interests. Optimization discussions of the components are presented in the following section. The consensus-value

compositions of SRM 610 (GeoReM, Max-Planck Institute Reference Materials<sup>1</sup>) and ARG-1 [24590-101-TSA-W000-0004-158-00002 (WTP-RPT-140), *Laser Ablation Study for High Level Waste and Melter Feed Characterization*] are summarized in Table 2.

**Table 2. Consensus-Value Composition (wt%) of ARG-1 and SRM 610**

Elements	ARG-1	SRM-610
Al	2.47	1.0812
B	2.65	0.0356
Ca	1.01	8.165
Cd	-	0.0259
Cr	0.068	0.0405
Fe	9.810	0.0458
K	2.220	0.0486
Li	1.48	0.0485
Mg	0.525	0.0465
Mn	1.470	0.0485
Na	8.31	9.941
Ni	0.817	0.0459
P	0.118	0.0343
S	-	0.0693
Sb	-	0.0369
Si	22.3	32.72
Sr	0.0034	0.0516
Th	-	0.0457
Ti	0.701	0.0434
Tl	-	0.0061
U	-	0.0462
Zn	0.0161	0.0456
Zr	0.104	0.0440

- Information is not reported

Optimization of the system required tuning of both the laser and the inductively coupled-atomic emission spectrometry (ICP-AES) units. The main goal was to achieve a good signal to background ratio for most of the analytes of interest. The laser ablates the sample to produce particles. The ablated particles are then transported in an argon stream to the plasma torch of ICP-AES where excitation of analytes takes place. The element specific wavelengths (lines) are measured by the ICP-AES spectrophotometer to quantify elements.

<sup>1</sup> GeoReM is a Max-Planck-Institute database for reference materials of geological and environmental interest, such as rock powders, synthetic, and natural glasses, as well as mineral, isotopic, biological, river water, and seawater reference materials.

Both laser ablation and ICP-AES parameters are important to achieve high quality data in accordance with the following references:

- a. DOE/RL-96-68, *Hanford Analytical Services Quality Assurance Requirements Documents (HASQARD)*.
- b. ATS-MP-1032, *222-S Laboratory Quality Assurance Plan*.
- c. PL-24590 QA00001, *Quality Assurance Project Plan for Testing Programs Generating Environmental Regulatory Data*.
- d. TFC-PLN-02, *Quality Assurance Program Description*.
- e. TFC-PLN-30, *CH2M HILL Analytical Technical Services Quality Assurance Program Plan*.

Section 3.2.1 addresses specific parameters tested and used for these studies.

### 3.2.1 Laser Optimization

The efficiency of particle generation is dependent on the laser parameters, i.e., beam energy, repetition rate, spot size, and scan rate. The system is equipped with a 266-nm ultraviolet (UV) laser beam, which is considered suitable for bulk analysis. It has been found that using a laser with output in the UV region of the spectrum, heating of the bulk sample is minimal and therefore vaporization of volatile constituents from the sample is avoided. Energy settings of 5%-100% can be chosen, and the energy at the sample can be measured by a built-in energy meter. For optimization an energy setting of 100% was used yielding energy of 8 mJ at the sample.

The spot size governs the amount of ablated particles produced. Larger beam sizes create larger craters and generate more particles. Various scientific articles on laser ablation suggest beam sizes ranging from 200  $\mu\text{m}$ -400  $\mu\text{m}$ :

- a. “Selection of Internal Standards for the Determination of Major and Minor Elements in Silicate Rocks and Limestones by Laser Ablation Inductively Coupled Plasma Atomic Emission Spectrometry” (Kanicky and Mermet 1997).
- b. “Use of Internal Standardization to Compensate for a Wide Range of Absorbance in the Analysis of Glasses by UV Laser Ablation Inductively Coupled Plasma Atomic Emission Spectrometry” (Kanicky et al. 1998).
- c. “Analysis of glass by UV laser ablation inductively coupled plasma atomic emission spectrometry. Part 1. Effects of the laser parameters on the amount of ablated material and the temporal behaviour of the signal for different types of laser” (Ducreux-Zappa and Mermet 1996).

However, the current laser system has a fixed beam diameter to produce a spot size of 150  $\mu\text{m}$  and generates enough particles to provide adequate signal on Hanford tank waste samples.

A typical repetition rate of 20 Hz was chosen for the best results based on the results of other studies, including SRNL and PNNL. The best signal and precision were obtained in the earlier studies using the repetition rate of 20 Hz.

The instrument options included using spot, line, and rastering sample patterns. A single spot will not give a steady signal over the duration of the analysis. Similarly, if the laser shots are fired on the same line repeatedly, the decrease of signal is obvious before the analysis is completed. Therefore, both spot and line patterns were deemed unsuitable. Instead a raster pattern was chosen because a representative sampling was desired to achieve reproducible results. A sufficient distance ( $\sim 200 \mu\text{m}$ ) was maintained between pattern lines to ensure that on the beam's second path, it would not cross over the original scanned line or debris from the first pass.

The scan rate was adjusted in conjunction with spot size. The available surface area on the sample and analysis time plays important roles in setting a scan speed. In this study a raster pattern was used that required ample surface on the sample during analysis. Although the instrument gave a choice of settings from 10  $\mu\text{m/s}$  to 1000  $\mu\text{m/s}$ , a 25  $\mu\text{m/s}$  scan rate was chosen for best results. This utilized (ablated) an area of approximately  $8.30 \text{ mm}^2$  during a typical analysis.

The results presented in Table 3 utilized the rastering sample pattern on SRM 610 glass. It is evident from the data that the drift was within acceptable range and the raster pattern suits well for achieving a steady-state signal.

**Table 3. Stability of Signal Using Raster Sample Pattern Over Time (SRM 610)**

Element and Wavelength (nm)	Concentration ( $\mu\text{g/g}$ )									% RSD
	0 hr	0 hr 5 min	0 hr 30 min	0 hr 45 min	1 hr	1 hr 15 min	1 hr 30 min	1 hr 45 min	2 hr	
Pb 220.353	342.1	433.6	436.1	452.8	439.8	434.2	450.4	428.3	427.6	2.42
Cd 214.441	240.5	237.8	240.6	251.5	250.0	245.3	256.8	229.7	230.1	3.85
Cr 359.349	421.7	405.7	383.6	426.8	414.6	366.9	367.3	372.0	378.8	6.15
Cu 224.700	312.7	449.6	386.4	384.1	360.9	361.0	401.2	321.1	312.0	12.17
La 429.655	438.2	457.6	431.0	441.6	438.0	431.1	447.4	421.3	407.4	2.38

RSD = relative standard deviation

The final operating parameters of laser ablation are provided in Table 4.

**Table 4. Laser Operating Parameters**

Laser wavelength	266 nm UV
Spot size ( $\mu\text{m}$ )	150 (largest aperture)
Laser power	100% setting ( $\approx 8 \text{ mJ}$ at sample)
Rate (Hz)	20
Method	Raster scan
Scan rate	25 $\mu\text{m/sec}$ (software setting of 25)

### 3.2.2 Inductively Coupled Plasma-Atomic Emission Spectroscopy Parameters

The LA-ICP-AES glove box prototype system integrated the laser unit to the HJY Ultima<sup>2</sup> ICP-AES. The optimization of the ICP-AES included the adjustment of radio frequency power and various argon gas flows (i.e., plasma, coating, auxiliary, and nebulizer). The nebulizer argon gas flow rate was also monitored to check for any fluctuation during the analysis. Initially, the specific operating conditions were set to the parameters utilized in the factory and site acceptance tests. The ICP-AES was allowed to warm up normally for 1 hour prior to analysis. In the WTP laboratory the instrument will be kept on all the time; therefore, no warm-up time will be required. A 90-second delay from the onset of the LA to ICP-AES signal processing was allowed for the stabilization in the plasma to occur. The peak integration time of 5 seconds was used for each analyte. The SRM 610 was ablated and the ICP-AES conditions were optimized to achieve optimum signal to background ratios for the analytes of interest. A summary of ICP-AES operating parameters is provided in Table 5. The argon flow to nebulizer was restricted in original instrument settings. This restriction was removed, and a gas flowmeter was installed to monitor actual nebulizer flow that allowed varying and optimizing the nebulizer gas flow during the optimization process.

**Table 5. Inductively Coupled Plasma-Atomic Emission Spectroscopy Operating Parameters**

Power (W)	1000
Plasma gas (L/minute)	12
Coating gas (L/minute)	G1-0.2
Auxiliary gas (L/minute)	0
Nebulizer pressure (bar)	3.73
Nebulizer flow (L/minute)	0.7
Stabilization time (seconds)	90

### 3.2.3 Inductively Coupled Plasma-Atomic Emission Spectroscopy Emission Lines

The HJY software has many lines available for each element, and factors such as detection limit, relative sensitivity, spectral interference, and signal to background ratios aid in selecting the best emission line for analysis of any given element. In a complex matrix where the possibility of interferences exists, choosing an interference-free line becomes extremely important. Therefore, analyzing multiple lines for a single element is advantageous to ensure valid data. Table 6 shows the lines that were chosen for this study. The selection was made on the basis of the vendor acceptance test and site acceptance test data. Most of the lines (except Al, B, Ca, P, and S) used in these tests were above 200 nm and did not require nitrogen purge of the ICP-AES optics. For Al, B, Ca, and P, alternate lines above 200 nm were also selected.

<sup>2</sup> HJY Ultima is a registered trademark of HORIBA Jobin Yvon Inc., Edison, New Jersey.

### 3.2.4 Particle Trap

Laser ablation can generate the particles of all sizes and shapes. Because larger particles may lead to erratic signal and poor sensitivity, they are not suitable for introduction into the plasma. The larger particles can also precipitate on the walls of the sample transfer tubing to introduce contamination. Therefore, a particle trap was introduced in the sample transfer line to trap larger particles. The presence of an in-line trap required increasing the purge time and also pre-ablation time. It was interesting to note (Table 7) that the particle trap improved the precision of the analysis. However, it had very little effect on the sensitivity.

**Table 6. Inductively Coupled Plasma-Atomic Emission Spectroscopy Wavelength Selection**

Element	Wavelength (nm)
Al	167.018; 226.346
B	181.724; 249.773
Ca	183.958; 317.933
Cd	226.502
Cr	205.571
Fe	259.940
K	766.490
Li	670.792
Mg	279.553
Mn	257.610
Na	589.592
Ni	231.096
P	178.221; 213.618
S	181.972
Sb	206.833
Si	252.411
Sr	215.284
Th	323.812
Ti	323.904
Tl	276.787
U	311.162
Zn	206.200
Zr	343.823

**Table 7. Effect of Particle Trap on the Precision of Analysis**

Element	% RSD without Particle Trap	% RSD with Particle Trap
Pb 220.353	4.76	0.86
Cd 214.441	4.04	0.83
Cr 359.349	2.83	1.13
Cu 224.700	3.85	0.72
La 429.655	2.13	0.90

### 3.2.5 Sample Analysis

The work performed at SRNL used a pre-ablation time of 45 seconds. The pre-ablation time ensures that the signal is at steady state prior to signal integration. The sample cell of this instrument is larger than laser ablation cells used in commercially available laser ablation instruments. This study not only concentrated on pre-ablation time but also optimized the gas purge time and wash time. The tube length to connect the laser sample cell to the ICP-AES torch was 22 ft. Both the large sample cell and long sample transfer tubing required purging of system and pre-ablation for a longer time to ensure that (a) the wash time between samples was sufficient to eliminate the cross contamination, (b) the purge gas flushed air from the laser ablation cell to an exit away from the plasma, and (c) the pre-ablation time was sufficient to stabilize the signal. Initially the purge time was set to 45 seconds, but when the sample trap was added to the transfer line, this time was increased to 90 seconds to account for the additional volume added to the system. The pre-ablation time was also increased to 90 seconds. While conducting these studies, the decay of the signal after the laser stopped ablating was also monitored. This was measured to determine the time needed to clear the sample out of the transfer tubing between analyses, thereby eliminating any possible sample contamination. The argon sweep gas was in bypass mode during coupon loading. After the coupon was placed in the laser ablation cell, the laser sample cell was purged for 90 seconds, and the argon flow was switched online to the ICP-AES. At this time the laser began ablating and sample ablation occurred. Argon flow through the sample cell and ICP-AES continued during the 90-second ICP-AES delay (pre-ablation) time, for a total sample cell purge of 3 minutes prior to ICP-AES data acquisition. The raster pattern established via computer control was used to ablate each sample.

Another parameter of interest was the number of replicates and integration time for each analyte. The total time of analysis for each wavelength varied depending on the ICP-AES used, specifically the integration time chosen. Since this ICP-AES is a sequential instrument, it measures analytes individually in sequence and takes more time compared to the simultaneous instrument used in studies at SRNL and PNNL. Increased replicates and integration time added to each element increased total measurement time. The data presented in this report utilized a 5-second integration time and three replicates for each analyte that yielded acceptable precision (Table 8).

### 3.2.6 Internal Standard

Laser ablation is different from wet analysis in that matrix matched calibration standards are not always available for analysis of wide variety matrix samples. However, use of an internal standard helps to compensate for the differences in ablation efficiencies of unmatched samples and calibration standards. Any element that resembles the behavior of the analyte of interest can be used as an internal standard. It can be added externally in the same quantity to both samples and calibration standards. An element already present in the sample can also be used as an internal standard if its concentration is known or can be determined by an independent technique. In the case of external addition, the element chosen as an internal standard ideally should not be

present in the sample, but if it is present its concentration should be known so it can be accounted for during data reduction.

**Table 8. Precision of Analysis of AY-102**

Element	Average Batch 1 (% RSD)	Average Batch 2 (% RSD)	Mean (% RSD)
Al 226.346	3.24	3.17	3.20
B 181.724	3.77	4.16	3.96
B 249.773	3.55	4.23	3.89
Ca 183.958	6.76	2.94	4.85
Ca 317.933	5.75	6.43	6.09
Cd 226.502	0.87	0.80	0.83
Cr 205.571	8.70	5.81	7.25
Fe 259.940	3.68	3.35	3.52
K 766.490	1.64	1.34	1.49
Li 670.792	3.01	4.43	3.72
Mg 279.553	7.52	12.91	10.22
Mn 257.610	5.00	4.60	4.80
Na 589.592	4.47	4.53	4.50
Ni 231.096	7.24	7.57	7.41
P 178.221	6.58	5.47	6.02
P 213.618	5.97	8.53	7.25
S 181.972	15.47	17.11	16.29
Sb 206.833	1.04	1.01	1.03
Si 252.411	3.77	5.63	4.70
Sr 215.284	9.65	9.39	9.52
Th 323.812	-	-	-
Ti 323.904	1.02	1.18	1.10
Tl 276.787	-	-	-
U 311.162	-	-	-
Zn 206.200	3.45	5.95	4.70
Zr 343.823	21.99	9.22	15.61

- Not analyzed

In this study, Sc was used as an internal standard. The samples and calibration standards containing 5% Sc were prepared and tested at SRNL and were tested in Phase II work (SRNL-SCS-2005-00019, *Candidates for RPP Glass Standards, May 2005 RPP Glass*; SRNL-SCS-2005-00052, *Measured Compositions of Candidates for WTP Glass Standards*). For accurate results, an internal standard was used with all the analyzed glasses.

### 3.2.7 Instrument Calibration

The instrument was calibrated using five well characterized glasses that were prepared at SRNL (WSRC-TR-2006-00003, *The Development of Laser Ablation-Inductively Coupled Plasma-Atomic Emission spectroscopy for the analysis of Hanford High level Waste: Phase II*). These nonradioactive glasses were composed to serve as calibration standards, which will encompass the range of the HLW glass that is to be made at the WTP. The composition of these standards

was confirmed by digestion and subsequent ICP-AES analysis. These glasses were spiked with Sc internal standard. The composition of the standards is given in Table 9.

**Table 9. Composition of Glass Standards (wt%)**

Element	RPP1	RPP2	RPP3	RPP4	RPP5
Al	1.124	0.774	2.078	3.323	0.753
B	2.709	1.789	1.544	1.147	4.554
Ca	1.505	1.853	0.731	0.391	0.099
Cd	0.534	1.628	1.321	0.394	0.035
Cr	0.068	0.226	0.041	0.116	0.034
Fe	6.524	3.507	4.970	2.709	13.741
K	0.855	0.091	1.594	3.312	0.091
Li	0.915	0.101	0.460	2.259	0.097
Mg	0.540	1.056	0.828	0.288	0.024
Mn	3.062	0.706	4.051	-	-
Na	9.798	6.882	6.179	5.306	14.844
Ni	1.038	2.059	0.684	0.299	0.008
P	0.312	0.576	0.273	0.189	0.092
Sb	0.710	1.971	1.303	0.459	0.084
Si	16.850	25.803	19.284	21.587	17.437
S	0.057	0.100	0.050	0.077	0.030
Sr	1.641	0.170	3.256	5.763	0.170
Th	-	-	-	-	-
Ti	1.164	0.546	1.740	0.066	0.060
Tl	-	-	-	-	-
U	-	-	-	-	-
Zn	2.384	0.720	3.264	0.080	0.800
Zr	2.370	0.060	1.620	6.230	0.090

- Not analyzed

It has been shown in “Quality of calibration in inductively coupled plasma atomic emission spectrometry” (Mermet 1994) that using more than four calibration standards yields a better calibration curve and coefficient of regression ( $r^2$ ). However, more statistical issues can develop with the use of a large number of standards. The  $r^2$  values generated from calibration curves are presented in Table 10. The elements and wavelengths are listed in the first column. The second column indicates the  $r^2$  values from the instrument output. In this case the instrument software calculated the  $r^2$  values from the calibration curves generated using all five calibration standards. The data presented in this report are primarily calculated by the instrument software based on these calibration curves.

The  $r^2$  values presented in the third column are based on data using four calibration standards that generated the best calibration curves. There is a significant improvement in the  $r^2$  values by excluding an outlier from the calibration data. It was noted that one calibration standard (RPP-2) did not have a smooth surface and visual analysis of that standard indicated some inclusions in that standard. Both sets of data are included to emphasize the importance of homogeneity and smooth surface. The poor fit for S may be attributed to its low concentration and sensitivity. For Si the poor fit may be due to clustering of calibration points.

**Table 10. Coefficients of Regression ( $r^2$ )  
from Calibration Curves**

Element and Wavelength (nm)	Instrument Output Five Calibration Standards	Best Fit Four Calibration Standards
Al 226.346	0.942	0.976
B 181.724	0.949	0.841
B 249.773	0.975	0.905
Ca 183.958	0.973	0.989
Ca 317.933	0.876	0.966
Cd 226.502	0.802	0.933
Cr 205.571	0.255	0.979
Fe 259.940	0.944	0.936
K 766.490	0.956	0.966
Li 670.792	0.957	0.985
Mg 279.553	0.830	0.916
Mn 257.610	0.839	0.997
Na 589.592	0.984	0.986
Ni 231.096	0.829	0.946
P 178.221	0.855	0.901
P 213.618	0.722	0.937
S 181.972	0.846	0.773
Sb 206.833	0.719	0.905
Si 252.411	0.728	0.753
Sr 215.284	0.971	0.953
Th 323.812	-	-
Ti 323.904	0.935	0.996
Tl 276.787	-	-
U 311.162	-	-
Zn 206.200	0.844	0.969
Zr 343.823	0.929	0.995

- Not analyzed

### 3.2.8 Detection Limits

Detection limits were estimated by using the lithium borate glass as the blank. A blank glass coupon was analyzed with each batch in a manner identical to the samples and the standard deviation ( $\sigma$ ) was estimated. The standard deviation was multiplied by three to calculate detection limits (Table 11) and converted to concentration on a wt% glass basis by dividing the instrument response by the slope of the calibration curve. These detection limits are much better than those obtained at SRNL (WSRC-TR-2005-00260 and WSRC-TR-2006-00003) using argon gas as a blank.

**Table 11. Estimated Detection Limits**

Element and Wavelength (nm)	Detection Limit (wt%)
Al 226.346	0.0127
B 181.724	0.0098
B 249.773	-
Ca 183.958	0.0156
Ca 317.933	0.0040
Cd 226.502	0.0019
Cr 205.571	0.0009
Fe 259.940	0.0277
K 766.490	0.0029
Li 670.792	-
Mg 279.553	0.0017
Mn 257.610	0.0195
Na 589.592	0.0091
Ni 232.096	0.0012
P 178.221	0.0005
P 213.618	0.0012
S 181.972	0.0027
Sb 206.833	0.0084
Si 252.411	0.0856
Sr 215.282	0.0035
Th 323.812	0.0074
Ti 323.904	0.0006
Tl 276.787	0.0004
U 311.162	0.0282
Zn 206.200	0.0045
Zr 343.823	0.0014

- Lithium and boron are the main constituents of the glass blank.

### 3.2.9 Radioactive Glass Sample and Analysis Sequence

WTP plans to collect four samples of feed before and eight samples after addition of glass former chemicals. Therefore, this study required analysis of two process batches of radioactive samples: one batch of four samples and another batch of eight samples. Since the task plan allowed use of previously made glass coupons, the AY-102 radioactive glass coupon prepared at SRNL was utilized in this study. The hot AY-102 glass contained Sc internal standard. The details of the glass coupon preparation and sample dose rates can be found in WSRC-TR-2006-00003.

Both analytical batches included blank and quality control samples (24590-WTP-RPT-OP-06-001, *LA-ICP-AES Analysis Method for Hanford Vitrification Process*). Analytical reference glass (ARG-1) was used as the laboratory control sample (LCS), and the lithium borate glass was utilized as a blank. The sequence of analysis for a batch of four samples requires seven analyses (ARG-1, AY-102, AY-102, Blank, AY-102, AY-102, ARG-1), and a batch of eight samples requires 11 analyses (ARG-1, AY-102, AY-102, AY-102, AY-102, Blank, AY-102, AY-102, AY-102, AY-102, ARG-1). Each AY-102 analysis was treated as a separate sample and was subjected to the

unloading and loading process in between each analysis to keep a running account of the analytical time.

### 3.2.10 Precision and Accuracy

The data from the analysis of AY-102 were evaluated for precision. The precision (Table 8) for most of the elements was about 5% relative standard deviation (RSD). The data presented in Table 8 are the average of 12 analyses in each batch. This indicates that the LA-ICP-AES analysis method produced consistent results and that the glass coupon preparation was well controlled and generated homogeneous product. The higher RSDs for some elements can be attributed to their poor sensitivity. Generally when concentration is small and sensitivity is low, higher deviations are seen. The consistency in precision indicates the stable performance of the laser unit.

The accuracy was evaluated for the scoping study with ARG-1 and AY-102. The ARG-1 was used as an LCS, and AY-102 was treated as an unknown sample. The analyses were conducted in the sequence as described in Section 3.2.9. The concentration calculations were made by the vendor-supplied instrument software.<sup>3</sup> The data generated by the ICP-AES were corrected using an internal standard correction.

The ICP-AES software generated data in terms of weight percent concentration at specified wavelengths. The internal standard correction was applied to account for differences in matrices of calibration standards and samples. Since Sc was present in both calibration standards and samples, a simplistic approach of direct ratio of internal standard concentration to analyte concentration was applied to achieve final results.

The ARG-1 results are summarized in Table 12. The accuracy of analysis was compared within  $\pm 15\%$  for a number of elements (Al, B, Fe, Li, Na, Ti), between 15% and 25% for K and Mn, and higher for P, Cr, Ca, Mg, Si, Ni. The elements in lower concentrations were not detected.

The LA-ICP-AES AY-102 coupon analysis results were evaluated relative to the wet chemistry ICP-AES results (Table 13). During the wet chemistry testing at SRNL (WSRC-TR-2005-00396, *Evaluation of Wet Chemical ICP-AES Elemental Analysis Methods Using both Actual and Simulated Hanford Waste Treatment Plant Samples – Phase II Report*, and WSRC-TR-2005-00169, *Evaluation of Wet Chemical ICP-AES Elemental Analysis Methods Using Simulated Hanford Waste Samples – Phase I Interim Report*) the results were generated by two different methods: cesium carbonate fusion and sodium peroxide fusion methods. The LA-ICP-AES results compared within  $\pm 15\%$  for Al, B, Ca, Fe, Li, Mg, Na, Ni, Si, and Ti. While the values for P and Cr were about 25% less than the SRNL reported values, the values for Mn and Zn were higher. The abundance of Cd, K, Sb, Sr, and Zr were below measurable level of the instrument and were not detected. The accuracy for S was not assessed because of the uncertainty in the reported value. The instrument calibration curve for Cr was not valid. The calculations were reprocessed manually to generate the numbers reported here. Additional work is required to confirm and validate the line selection for Cr.

---

<sup>3</sup> Activa Analyst ver. 5.4 is a registered trademark of HORIBA Jobin Yvon Inc., Edison, New Jersey.

**Table 12. Reported and Analyzed Concentrations (wt%)  
in ARG-1 Glass Coupon**

Element and Wavelength (nm)	Analyzed Concentration	PNNL Reported Concentration	% Difference
Al 226.346	2.697	2.47	9.19
B 181.724	2.748	2.65	3.70
B 249.773	3.007	2.65	13.47
Ca 183.958	1.900	1.01	88.12
Ca 317.933	1.601	1.01	58.51
Cd 226.502	-	-	-
Cr 205.571	0.048	0.068	28.75
Fe 259.940	8.691	9.81	11.41
K 766.490	1.736	2.22	21.80
Li 670.792	1.572	1.48	6.22
Mg 279.553	0.927	0.525	76.57
Mn 257.610	1.763	1.47	19.93
Na 589.592	7.873	8.31	5.26
Ni 232.096	1.688	0.817	106.61
P 178.221	0.267	0.118	126.27
P 213.618	0.085	0.118	27.97
S 181.972	0.060	-	-
Sb 206.833	-	-	-
Si 252.411	28.475	22.3	27.69
Sr 215.282	-	0.0034	-
Th 323.812	-	-	-
Ti 323.904	0.794	0.701	13.27
Tl 276.787	-	-	-
U 311.162	-	-	-
Zn 206.200	-	0.016	-
Zr 343.823	-	0.104	-

- Not detected

**Table 13. Analyzed and Reported Elemental Concentrations (wt%)  
in AY-102 Glass Coupon**

Element and Wavelength (nm)	Analyzed Concentration	Reported Concentration			
		Na <sub>2</sub> O <sub>2</sub> Fusion	% Difference	Cs Carbonate Digestion	% Difference
Al 226.346	3.671	3.230	13.6	3.090	18.8
B 249.773	3.446	3.170	8.7	2.980	15.6
Ca 183.958	0.743	0.672	10.5	0.414	79.4
Cd 226.502	-	0.024	-	0.044	-
Cr 205.571	0.154	0.244	31.25	0.208	25.96
Fe 259.940	8.547	9.600	11.0	9.650	11.4
K 766.490	-	6.530	-	5.390	-
Li 670.792	1.399	1.620	13.6	1.510	7.3
Mg 279.553	0.090	0.106	15.4	0.095	5.6
Mn 257.610	2.789	2.050	36.0	2.070	34.7
Na 589.592	9.516	-	-	8.640	10.1
Ni 232.096	0.521	0.573	9.1	0.468	11.3
P 178.221	0.796	1.010	21.2	1.070	25.7
S 181.972	0.054	<0.142	-	<0.193	-
Sb 206.833	-	0.446	-	0.435	-
Si 252.411	27.060	23.800	13.7	24.200	11.8
Sr 215.282	-	0.517	-	0.371	-
Th 323.812	-	0.250	-	0.341	-
Ti 323.904	0.073	0.074	0.54	0.063	16.3
Tl 276.787	-	2.530	-	2.510	-
U 311.162	-	1.960	-	1.590	-
Zn 206.200	0.997	0.690	44.4	0.684	45.7
Zr 343.823	-	-	-	0.391	-

- Not detected

Because of the lack of calibration curves, the concentration for Th, U, and Tl were not calculated by the instrument directly as for other elements. However, it was possible to calculate these concentrations by using other approaches such as surrogate calibration. The data presented in Table 14 were calculated using Ti as a surrogate element. The Th/Ti, Tl/Ti, and U/Ti ratios were derived from National Institute of Standards and Technology SRM 610 glass, and the ratios were applied to the Ti calibration curve for concentration calculations. The instrument response values were used directly in these calculations. Because of uncertainty in reported value of Tl in SRM 610, the data for this element turned out to be very low as compared to the reported value. For comparison purposes, Zn data were also calculated using the surrogate calibration, and the results are comparable to the SRNL reported values (Table 13).

**Table 14. Analyzed and Reported Concentrations (wt%) of Th, Tl, and U in AY-102 Glass**

Element and Wavelength (nm)	Analyzed Value Laser Ablation	Reported Concentration	
		Na <sub>2</sub> O <sub>2</sub> Fusion	Cs Carbonate Digestion
Th	323.812	0.53	0.25
Tl	276.787	0.04	2.53
U	311.162	1.08	1.96
Zn	206.200	0.61	0.69

### 3.2.11 Operator and Day Variability

The scoping study required that the analyses be performed by different chemists on three different days. The objective of this study was to demonstrate the robustness of the technique to support the vitrification process. When the WTP plant will be running 24/7, the different analysts will perform analyses on different shifts. To be consistent with the task plan, the first batch of four AY-102 samples was analyzed by analyst 1. In the second batch of eight AY-102 samples, the first four samples were analyzed by analyst 1, and the remaining four samples were analyzed by analyst 2. The whole set was repeated to check the reproducibility of the analysis. The data presented in Table 15 indicate that the data obtained by two analysts on three different days was comparable. The method performance meets the day-to-day variability and requirements defined in Appendix A.

### 3.2.12 Turnaround Time Study

The TAT study evaluated total time required from sample receipt to data generation and included the following steps: (a) sample preparation, (b) analysis, and (c) data reduction. The primary objective of the LA-ICP-AES testing was to determine the sample TAT for performing sample preparation and analysis inside the hot cell. Times were not recorded for the following operational activities that did not directly influence the ability to meet the target TAT because in an operational mode these activities are assumed to be performed prior to receipt of samples:

- a. Weighing of fusion flux in vials and transferring vials to the hot cell.
- b. Preparing the calibration standard, blank, and LCS glass coupons and transferring them to the hot cell.
- c. Staging laboratory supplies at the work station that are needed for procedure execution.
- d. Initializing and warm-up of laser ablation unit and ICP-AES.
- e. Calibrating the LA-ICP-AES.

The LA-ICP-AES time study results were obtained from analytical work that mimics the WTP production laboratory's analysis of the HLW samples. The summary of the time required for each category and substeps is given in Table 16.

**Table 15. Elemental Concentration (wt%) of AY-102 Analyzed by Different Operators on Different Days**

Element and Wavelength (nm)	Day 1 Operator 1	Day 2 Operator 1	Day 2 Operator 2	Day 3 Operator 1	Day 3 Operator 1	Day 3 Operator 2	Average $\pm \sigma$	Percent Variation
Al 226.346	3.893	3.288	4.017	3.303	3.258	4.265	$3.671 \pm 0.442$	12.0
B 181.724	4.061	3.367	4.064	3.218	5.457	4.020	$4.031 \pm 0.792$	19.7
B 249.773	4.138	3.051	3.766	3.038	2.972	3.709	$3.446 \pm 0.489$	14.2
Ca 183.958	0.810	0.541	0.773	0.583	1.048	0.700	$0.743 \pm 0.182$	24.6
Ca 317.933	0.419	0.380	0.432	0.308	0.306	0.417	$0.377 \pm 0.057$	15.1
Cd 226.502	-	-	-	-	-	-	-	-
Cr 205.571	0.522	0.292	0.491	0.393	0.557	0.714	$0.495 \pm 0.144$	29.2
Fe 259.940	9.774	7.613	8.435	7.220	8.704	9.537	$8.547 \pm 1.015$	11.9
K 766.490	-	-	-	-	-	-	-	-
Li 670.792	1.432	1.456	1.526	1.132	1.500	1.348	$1.399 \pm 0.144$	10.3
Mg 279.553	0.109	0.086	0.117	0.056	0.054	0.116	$0.090 \pm 0.029$	32.5
Mn 257.610	3.181	2.342	2.975	2.291	2.707	3.237	$2.789 \pm 0.411$	14.7
Na 589.592	8.950	9.452	9.019	8.733	10.885	10.057	$9.516 \pm 0.818$	8.6
Ni 232.096	0.564	0.301	0.722	0.505	0.355	0.680	$0.521 \pm 0.169$	32.5
P 178.221	0.689	0.639	0.899	0.608	1.117	0.821	$0.796 \pm 0.193$	24.2
P 213.618	0.506	0.331	0.570	0.366	0.337	0.497	$0.435 \pm 0.102$	23.5
S 181.972	0.077	0.059	0.065	0.031	0.054	0.036	$0.054 \pm 0.017$	32.4
Sb 206.833	-	-	-	-	-	-	-	-
Si 252.411	31.574	23.897	28.766	24.107	26.222	27.797	$27.060 \pm 2.941$	10.9
Sr 215.282	-	-	-	-	-	-	-	-
Th 323.812	-	-	-	-	-	-	-	-
Ti 323.904	0.082	0.078	0.067	0.066	0.075	0.073	$0.073 \pm 0.006$	8.1
Tl 276.787	-	-	-	-	-	-	-	-
U 311.162	-	-	-	-	-	-	-	-
Zn 206.200	1.011	0.770	1.055	0.929	1.027	1.187	$0.997 \pm 0.139$	14.0
Zr 343.823	-	-	-	-	-	-	-	-

- Not detected (below detection limit)

**Table 16. Turnaround Time Study**

General Steps	Activity	Time
Sample preparation	Details in Table 1	1 hour 45 minutes
	Estimated fusion time for batch 1 (four samples)	2 hours 45 minutes
	Estimated fusion time for batch 2 (eight samples)	3 hours 45 minutes
Sample analysis	Load sample	2 minutes
	Purge laser cell	1.5 minutes
	Stabilize ICP-AES	1.5 minutes
	Analysis	10 minutes
	Total analysis time/sample	15 minutes
	Time for analysis of batch 1	1 hour 45 minutes
	Time for analysis of batch 2	2 hours 45 minutes
Data reduction/verification	Internal standard Correction	2 hours
	<b>Grand total for batch 1</b>	<b>6 hours 30 minutes</b>
	<b>Grand total for batch 2</b>	<b>8 hours 30 minutes</b>

The time for fabricating one glass coupon was 1 hour 45 minutes (Table 1). The first batch will require preparation of four glass coupons. If the WTP acquires a furnace large enough to accommodate eight samples, the sample drying, fusion, and cooling for four samples of batch 1 can be done in parallel. Similarly, the eight samples of batch 2 can be dried, fused, and cooled at the same time. The additional time required to process each sample will be only for remaining steps (i.e., weighing the sample aliquot, mixing fusion flux, etc.) of the sample preparation procedure. Table 1 indicates that these remaining steps can be completed in 15 minutes. This will add an extra hour to the batch 1 samples and 2 hours to the batch 2 samples. Therefore, the time to complete the sample preparation for batch 1 and batch 2 can be estimated to be 2 hours 45 minutes and 3 hours 45 minutes, respectively.

The analysis time for each sample, as indicated in Table 16, is 15 minutes. According to Section 3.2.8, batch 1 is comprised of a total of seven analyses and batch 2 of 11 analyses. Therefore, the analysis of batch 1 was completed in 1 hour 45 minutes and batch 2 in 2 hours 45 minutes. The data reduction and verification for each batch can be accomplished in 2 hours time. The data reduction time for the Th, Tl, and U calculations was excluded as these activities will be automated when the instrument is installed at WTP. The overall TAT for a process batch of four samples is estimated at 6 hours 30 minutes and for a batch of eight samples is 8 hours 30 minutes. Both TATs are less than 9 hours and meet the WTP requirement.

### 3.2.13 Analysis of 241-AN-102

The applicability of the method was reassessed again by analyzing a radioactive waste glass sample prepared from 241-AN-102 tank material. The 241-AN-102 material was converted to a glass coupon as described in Section 3.1 and then split into two sections for analysis. One part was analyzed by Advanced Technologies and Laboratories International, Inc. (ATL) using a conventional dissolution followed by the standard laboratory ICP-AES method; and the other part was analyzed using the LA-ICP-AES method in Appendix F (ATS-LT-505-105, “222-S Laboratory Laser Ablation-Inductively Coupled Plasma Atomic Emission Spectrometry Analysis”). A glass sample prepared from 241-AN-102 and an ARG-1 glass standard provided by SRNL were analyzed using both approaches. The glass samples analyzed using the standard laboratory methods were ground into small particles of glass prior to analysis. ATL prepared and analyzed the 241-AN-102 and ARG-1 glass samples in accordance with procedure LA-505-114, “Microwave Assisted Acid Digestion of Air Filter Media, Wipes, and Bulk Materials for Analysis by Inductively Coupled Plasma.” Subsequent analyses were performed by ICP-AES using procedure LA-505-161, “Inductively Coupled Plasma (ICP) Emission Spectrometric Method for the Thermo Jarrell Ash Type 61E.”

The LA-ICP-AES data were obtained using procedure ATS-LT-505-105 (see Table 17). The analytical results obtained by LA-ICP-AES showed some of the elements of interest were below the method detection limit; however, the results for the other elements were consistently higher than ATL data. The discrepancy may indicate that the test recipe for producing glass from Hanford tank waste needs to be modified to increase sample mass in the glass matrix. This would increase the LA-ICP-AES method accuracy. Additionally improving the method used for introducing the internal standard into the glass matrix will also improve the method accuracy.

## 4. QUALITY ASSURANCE AND SAFETY

This task was conducted following the guidelines established by APD within the administrative structure of the 222-S Laboratory. The work was performed using the Integrated Safety Management System approach. The work was completed under the WRPS contract with the U.S. Department of Energy, Office of River Protection. The WRPS contract specifies that WRPS operate a quality assurance program based on the requirements of Title 10, *Code of Federal Regulations*, Part 830, “Nuclear Safety Management,” Subpart A (10 CFR 830, Subpart A); DOE O 414.1C, *Quality Assurance*, for facilities and projects within the scope of work; and NQA-1-2004, “Quality Requirements for Nuclear Facility Applications.” (Contract No. DE-RP27-07RV14800, Section C.3.2.4 Quality)

All employees are responsible for performing work in accordance with the documented requirements. Those employees performing oversight and verification have the authority and responsibility to identify quality problems, recommend solutions, and verify implementation of effective corrective actions. Employees have the authority to stop work when they determine a situation represents an imminent hazard that places their personal safety, the safety of their coworkers, or the environment at risk.

**Table 17. LA-ICP-AES and ICP-AES Method Comparison (wt%)**

Elements	LA-ICP-AES (wt%)	ICP-AES (wt%)	LA-ICP-AES (wt%)	ICP-AES (wt%)
	Tank 241-AN-102		ARG-1	
Al	0.58	0.175	4.58	1.65
B	37.31	20.90	2.45	2.51
B	46.03	20.90	2.99	2.51
Ca*	<	<	2.18	0.898
Ca*	<	<	2.30	-
Cd	<	<	<	<
Cr	<	0.217	0.09	0.0635
Fe	1.00	0.0056	11.66	9.11
K	<	0.171	3.06	2.42
<b>Li</b>	<b>27.51</b>	<b>7.97</b>	<b>2.42</b>	<b>1.70</b>
Mg	<	<	1.28	0.437
Mn	<	<	2.77	1.32
Na	11.72	2.58	10.22	8.84
Ni	<	<	2.25	0.750
P <sup>‡</sup>	0.02	<	0.18	<
P <sup>‡</sup>	<	<	0.07	-
S	0.27	0.0795	0.03	<
Sb	<	<	<	<
Si	<	3.57	31.20	21.3
Sr	<	<	<	0.00297
Th	<	<	<	<
Ti	0.06	<	1.03	0.5960
Tl	<	<	<	<
U	<	<	<	<
Zn	<	<	<	0.0163
Zr	<	<	<	0.0866

\* More than one emission line measurement obtained for LA-ICP-AES data.

< The concentration in the sample was less than the method detection limit.

The installation of the LA-ICP-AES system required significant preparation including reduction of radiological inventory to as low as reasonably achievable (ALARA), job planning with worker involvement, and joint review committee approvals. System mockups and dry runs were performed as part of workforce training.

Analytical tests were performed in accordance with HNF-SD-CP-QAPP-016, *222-S Laboratory Quality Assurance Plan*, and DOE/RL-96-68, *Hanford Analytical Services Quality Assurance Requirements Documents (HASQARD)*. No analytical data were generated to support WTP process use or any waste characterization. The information present here is limited to the assessment of the applicability of this technology to address future technology needs. The information in this report does not support LA-ICP-AES method validation. Method validation was not within the authorized scope of work for this project.

The LA-ICP-AES instrumentation provided by WTP was successfully received and adapted to the 11A hot cells. The APD group at the 222-S Laboratory has demonstrated acceptable TAT of less than 9 hours and the LA-ICP-AES system has shown to provide sufficient data sensitivity and accuracy to meet the needs of WTP.

## 5. DISCUSSION AND RECOMMENDATIONS

The LA-ICP-AES instrumentation provided by WTP was successfully received and adapted to the 11A hot cells. The APD group at the 222-S Laboratory has demonstrated acceptable TAT of less than 9 hours. The procedure was shown to provide sufficient data sensitivity, accuracy, and precision of the LA-ICP-AES method. This includes development of an in-cell glass fusion procedure for the preparation of melter feed into a glass matrix that can be analyzed. The LA-ICP-AES method does offer WTP the ability to receive and analyze feed material in one shift as a process control analysis for the feed to the glass melter.

This study disclosed some areas where the equipment and analytical methodology should receive additional optimization:

a. Design Improvements:

1. As noted in the report, the torch positioning mechanism became jammed. The problem remained hidden for some time as the adjustment for the horizontal position is set and moved at only one point. Using this design can result in an operator believing the torch is moving in a straight horizontal line, but if the mechanism is jammed, the torch is actually being moved in an arc due to increasing tension on one side of the adjustment mechanism. This design issue can be prevented by redesigning the adjustment mechanism to engage the torch support at two opposing positions.
2. The glove box was designed with a load-in/load-out port that is designed to always push material into the glove box. Material can be loaded out only by cutting it up into small pieces and bagging out, but to replace the bag with a new one required the retaining ring and unused bag to be pushed into the glove box. This makes the load-in/load-out process very inefficient and always leaves waste residue in the working space inside the glove box. The original design of a “French Can” port or a double-door pass-through would resolve this issue.
3. The system was operated at the 222-S Laboratory in two different configurations: first as a glove box as designed and secondly installed in a laboratory hood. The hood configuration was set by removing two gloves from the glove ports and adjusting the flow rates for air entering the enclosure. There were no issues with dose rates or contamination in either configuration, and the change had no impact on the performance of the LA-ICP-AES. Operating the system in the fume hood configuration greatly simplifies standard operations such as maintenance or waste management. The fume hood installation should be evaluated for use at the WTP laboratory.

b. Calibration and instrument sensitivity:

1. The wavelength selection to this point is limited to the vendor-selected wavelengths used in the original vendor tests. Method performance can be improved by optimization of the wavelength selection to the matrix being analyzed. Additional testing and optimization of alternate wavelengths should be performed.
2. A proven method for producing glass standards in the waste matrices that will be processed at WTP need to be validated. The prepared standards should include a wider range of elements and compositions for bracketing the analysis of Hanford tank waste vitrification process samples.
3. It may be possible to calibrate the LA-ICP-AES using liquid standards and understanding the physics of the aerosol transport. The method currently uses internal tracers to monitor the aerosol so this change may be implemented simply by adjusting the torch arrangement to introduce water to the plasma while the laser is in operation. The impact of such a change should be investigated.
4. It was noticed that processing data offline can in some cases generate better data fits. Validation of offline data calculations becomes necessary for process support. More work is required to standardize and automate data processing and the methodology used for internal standard corrections.
5. It has been suggested that a pressed pellet sample preparation similar to what is currently used in X-ray sample analysis may be able to replace the glass fusion sample preparation used in this study. If such a sample could be successfully ablated, there would be time saved in the sample preparation steps. Additional investigation would be required to study and evaluate this option.

Overall the results obtained from the LA-ICP-AES analysis of the radioactive AY-102 glass are satisfactory. The adaptation of the developed method (for hot cell testing using radioactive samples) successfully demonstrated the acceptance of selected technology for meeting the rapid TAT requirements for monitoring the vitrification process.

## 6. REFERENCES

7S110-MFM-07-096, 2007, "Preparation of Glass Coupons from Tank Simulant" (interoffice memorandum from M. F. Marcus to C. M. Seidel, January 25), CH2M HILL Hanford Group, Inc., Richland, Washington.

10 CFR 830, "Nuclear Safety Management," Subpart A—Quality Assurance Requirements, *Code of Federal Regulations*, as amended.

24590-101-TSA-W000-0004-153-00005 (WTP-RPT-139), 2005, *Conventional Non-Dilute West Chemistry Dissolution/ICP-AES Time Study*, Battelle-Pacific Northwest Division (PNWD), Richland, Washington (proprietary).

24590-101-TSA-W000-0004-158-00002 (WTP-RPT-140), 2005, *Laser Ablation Study for High Level Waste and Melter Feed Characterization*, Battelle-Pacific Northwest Division (PNWD), Richland, Washington (proprietary).

24590-WTP-RPT-OP-06-001, Rev 0, *LA-ICP-AES Analysis Method for Hanford Vitrification Process*, Bechtel National, Inc., Richland, Washington.

ATS-MP-1027, *Management Plan for Waste Treatment Plant Project Work Performed by Analytical Technical Services*, CH2M HILL Hanford Group, Inc., Richland, Washington.

ATS-MP-1032, *222-S Laboratory Quality Assurance Plan*, Washington River Protection Solutions LLC, Richland, Washington.

DOE O 414.1C, *Quality Assurance*, U.S. Department of Energy, Washington, D.C.

DOE/RL-96-68, *Hanford Analytical Services Quality Assurance Requirements Documents (HASQARD)*, U.S. Department of Energy, Richland Operations Office, Richland, Washington, as amended.

Ducréux-Zappa, M., and J.-M. Mermet, 1996, "Analysis of glass by UV laser ablation inductively coupled plasma atomic emission spectrometry. Part 1. Effects of the laser parameters on the amount of ablated material and the temporal behaviour of the signal for different types of laser," *Spectrochim. Acta Part B*, Vol. 51, pp. 321-332.

HNF-SD-CP-QAPP-016, 2005, *222-S Laboratory Quality Assurance Plan*, Rev. 9, CH2M HILL Hanford Group, Inc., Richland, Washington.

Kanicky, V., and J.-M. Mermet, 1997, "Selection of Internal Standards for the Determination of Major and Minor Elements in Silicate Rocks and Limestones by Laser Ablation Inductively Coupled Plasma Atomic Emission Spectrometry," *Appl. Spectro.*, Vol. 51, Issue 3, pp. 332-336.

Kanicky, V., V. Otruba, and J.-M Mermet, 1998, "Use of Internal Standardization to Compensate for a Wide Range of Absorbance in the Analysis of Glasses by UV Laser Ablation Inductively Coupled Plasma Atomic Emission Spectrometry," *Appl. Spectro.*, Vol. 52, Number 5, pp. 638-642.

Mermet, J.-M., 1994, "Quality of calibration in inductively coupled plasma atomic emission spectrometry," *Spectrochim. Acta Part B*, Vol. 49, Issues 12-14, pp. 1313-1324.

NQA-1-2004, *Quality Requirements for Nuclear Facility Applications*, American Society of Mechanical Engineers, New York, New York

PL-24590 QA00001, 2001, *Quality Assurance Project Plan for Testing Programs Generating Environmental Regulatory Data*, Rev 0, Bechtel National, Inc., Richland, Washington.

SRNL-SCS-2005-00019, 2005, *Candidates for RPP Glass Standards RPP Glass, Rev 0*, Westinghouse Savannah River Company, Aiken, South Carolina.

SRNL-SCS-2005-00052, 2005, *Measured Compositions of Candidates for WTP Glass Standards (U)*, Rev 0, Westinghouse Savannah River Company, Aiken, South Carolina.

Task Order 2005-003, June 2005, "Laser Ablation/Inductively Coupled Plasma-Atomic Emission Spectroscopy (LA-ICP-AES) Study at CHG-222S using Hot-Cell Glovebox Prototype System," CCN: 122474, Bechtel National, Inc., Richland, Washington.

TFC-PLN-02, Rev. B-3, *Quality Assurance Program Description*, CH2M HILL Hanford Group, Inc., Richland, Washington.

TFC-PLN-30, Rev. A-2, *CH2M HILL Analytical Technical Services Quality Assurance Program Plan*, CH2M HILL Hanford Group, Inc., Richland, Washington.

WSRC-TR-20005-00169 (SRNL-RPP-2005-00023), SCT-M0SRLE60-00-145-00010, 2005, *Evaluation of Wet Chemical ICP-AES Elemental Analysis Methods Using Simulated Hanford Waste Samples – Phase I Interim Report (U)*, Rev 0A, Westinghouse Savannah River Company, Aiken, South Carolina.

WSRC-TR-2005-00260 (SRNL-RPP-2005-00038), SCT-M0SRLE60-00-216-00002, 2005, *The Development of Laser Ablation-Inductively Coupled Plasma-Atomic Emission Spectroscopy for the Analysis of Hanford High Level Waste: Phase 1*, Rev 0A, Westinghouse Savannah River Company, Aiken, South Carolina.

WSRC-TR-2005-00396 (SNRL-RPP-2005-00056), SCT-M0SRLE60-00-145-00019, 2005, *Evaluation of Wet Chemical ICP-AES Elemental Analysis Methods Using both Actual; and Simulated Hanford Waste Treatment Plant Samples – Phase II Report*, Rev 0A, Westinghouse Savannah River Company, Aiken, South Carolina.

WSRC-TR-2006-00003 (SRNL-RPP-2006-00002), SCT-M0SRLE60-00-216-00002, 2006, *The Development of Laser Ablation-Inductively Coupled Plasma-Atomic Emission Spectroscopy for the Analysis of Hanford High Level Waste: Phase II*, Rev 0A, Westinghouse Savannah River Company, Aiken, South Carolina.